

Fig. 1

2/42

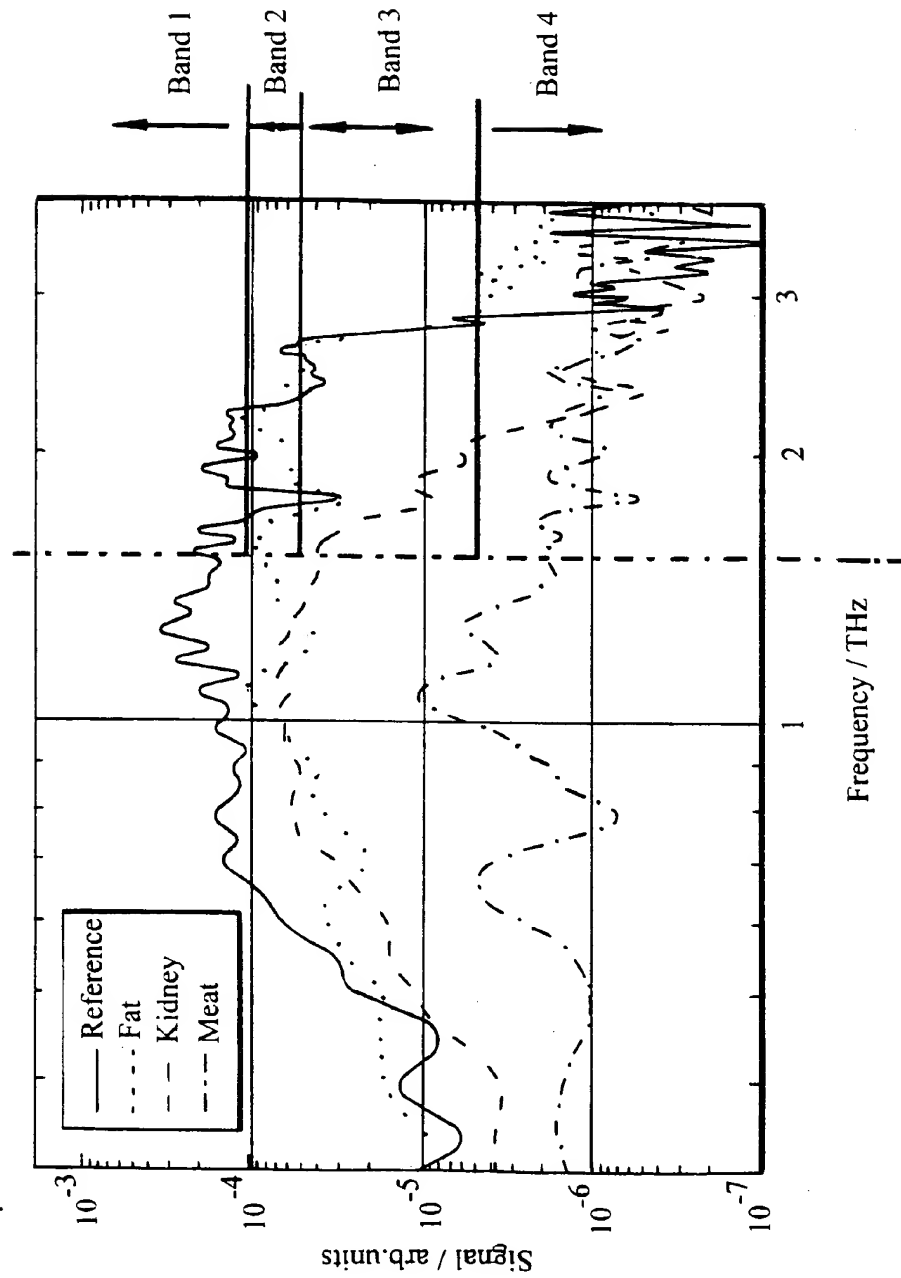


Fig. 2

SUBSTITUTE SHEET (RULE 26)

3/42

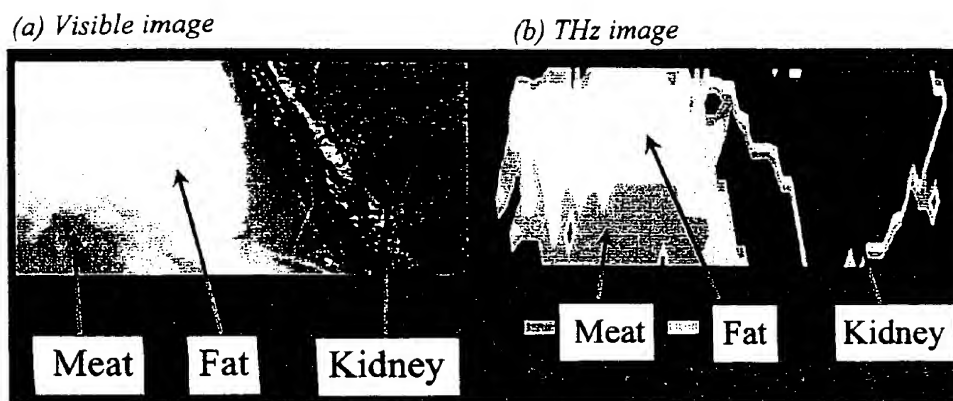


Fig. 3

4/42

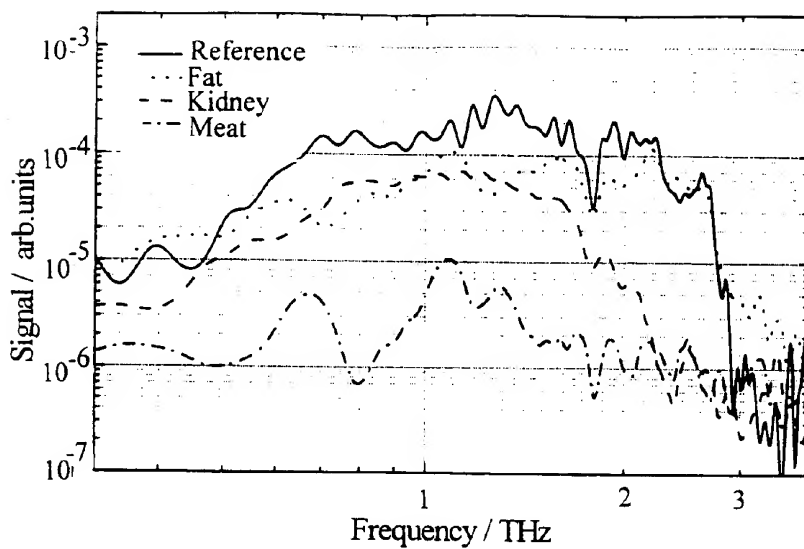


Fig. 4

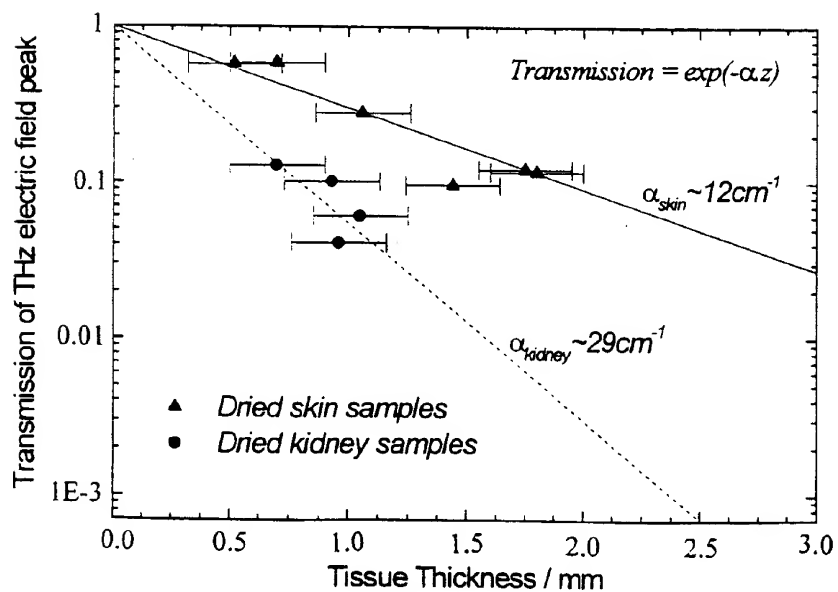


Fig. 5

5/42

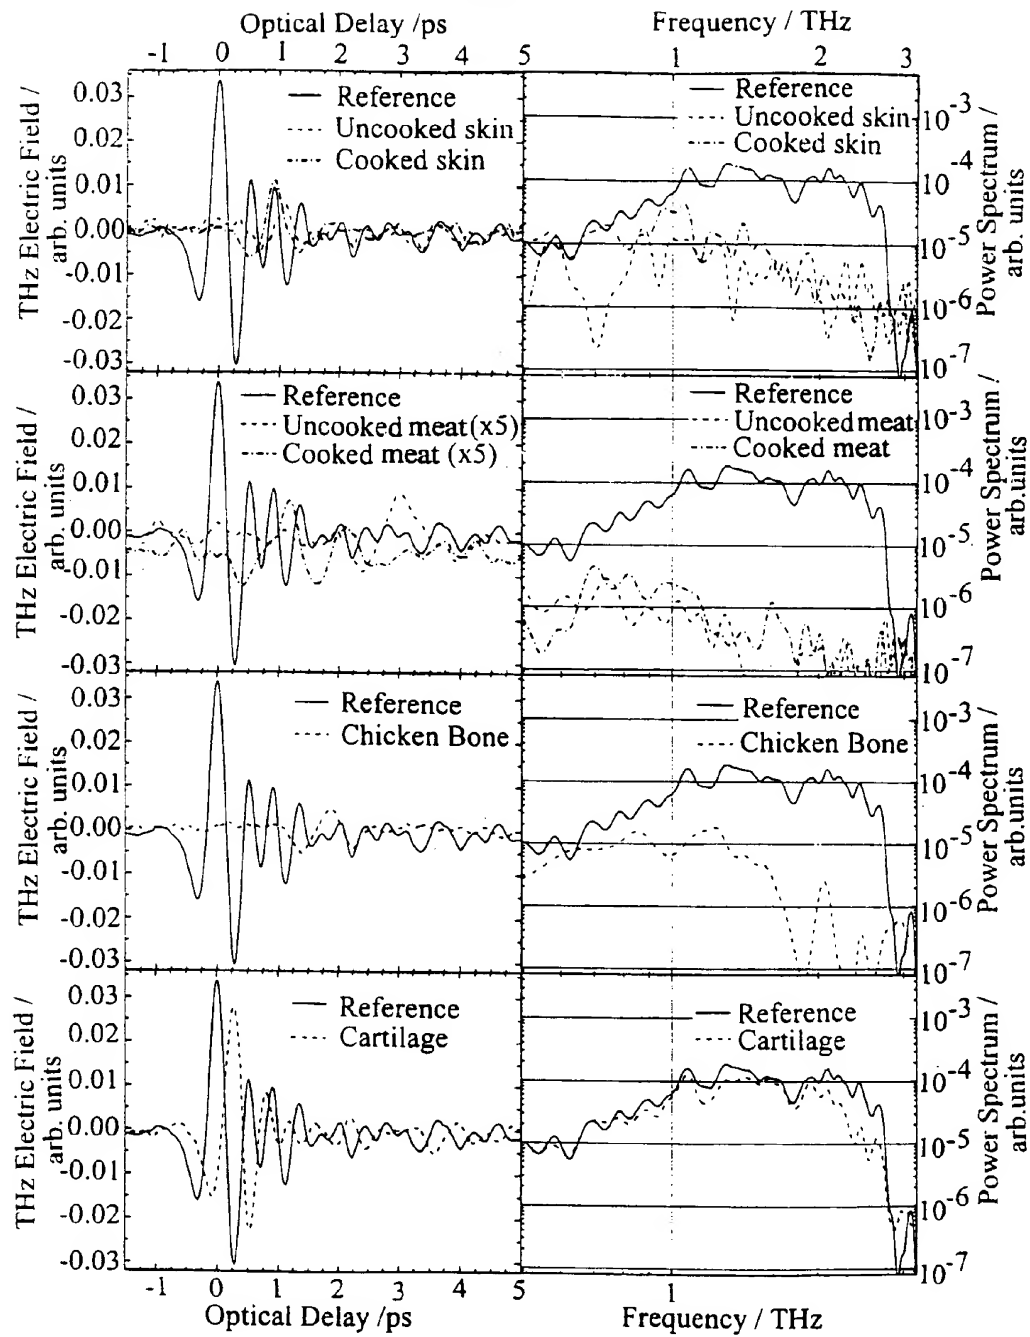


Fig. 6

6/42

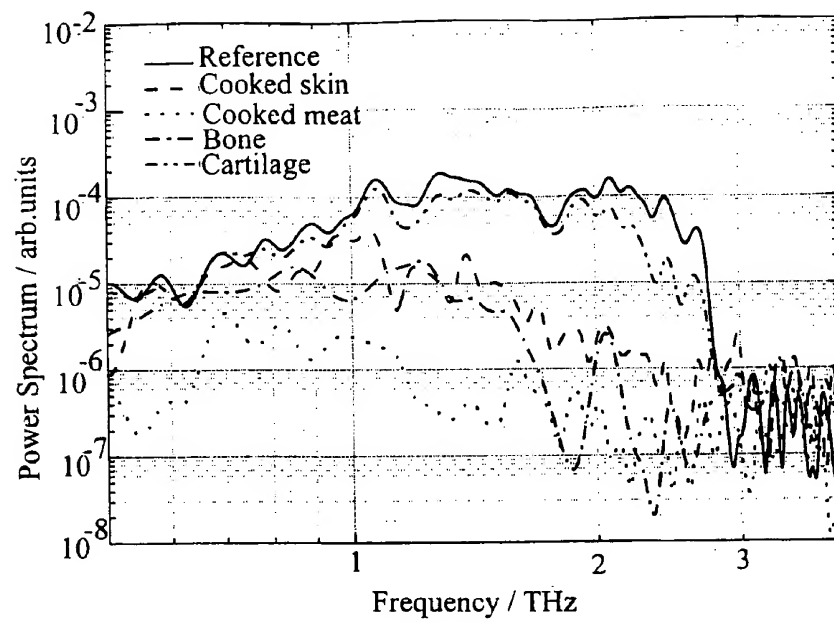


Fig. 7

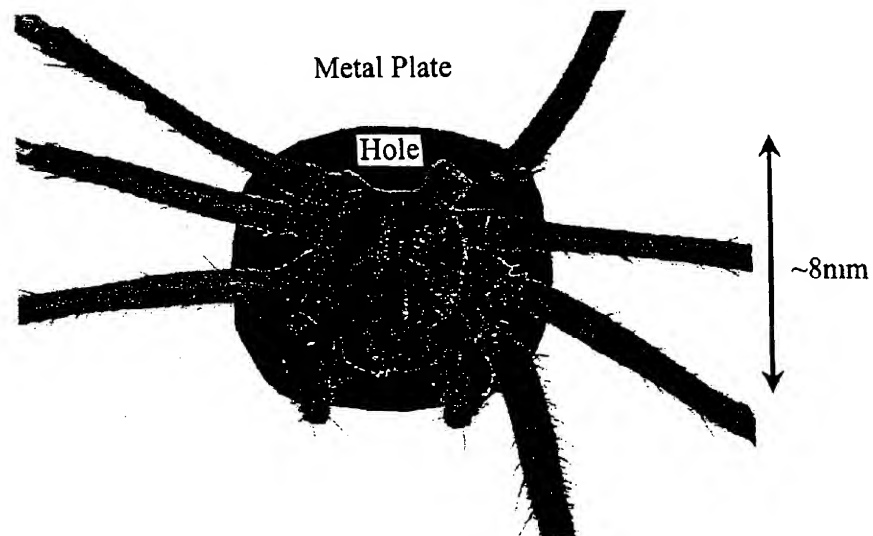


Fig. 8

7/42

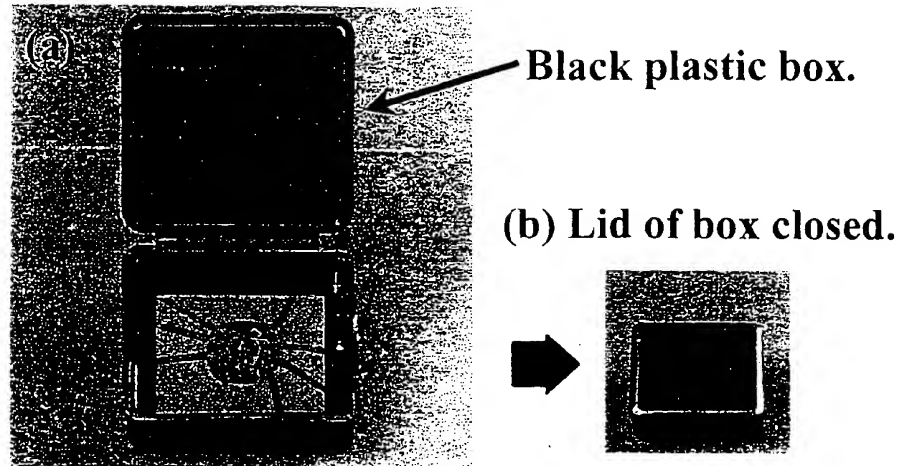


Fig. 9

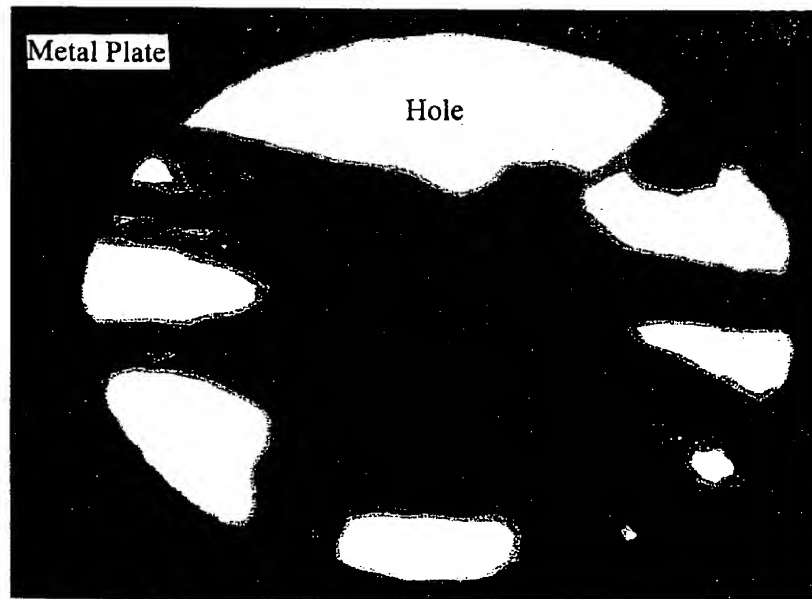


Fig. 10

8/42

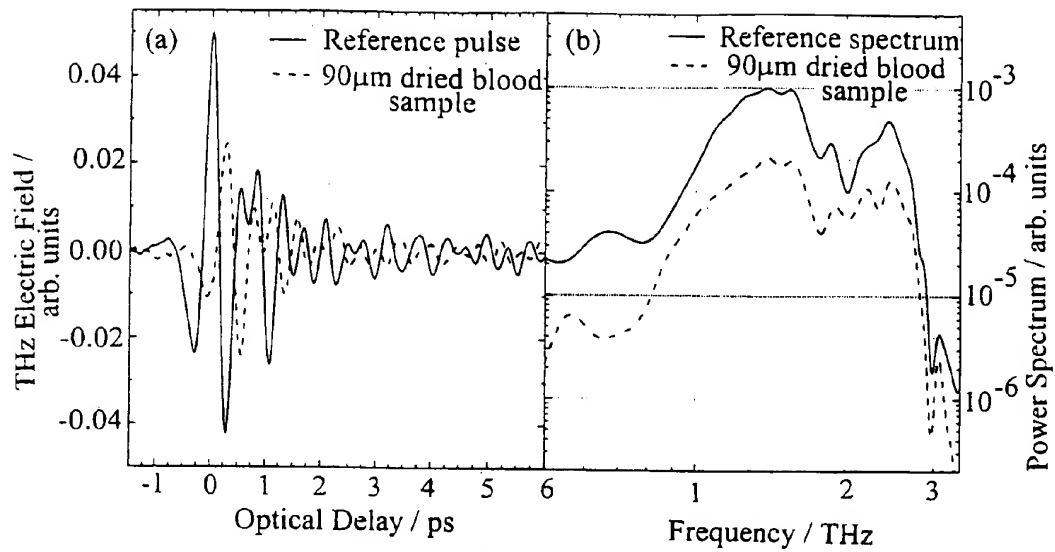


Fig. 11

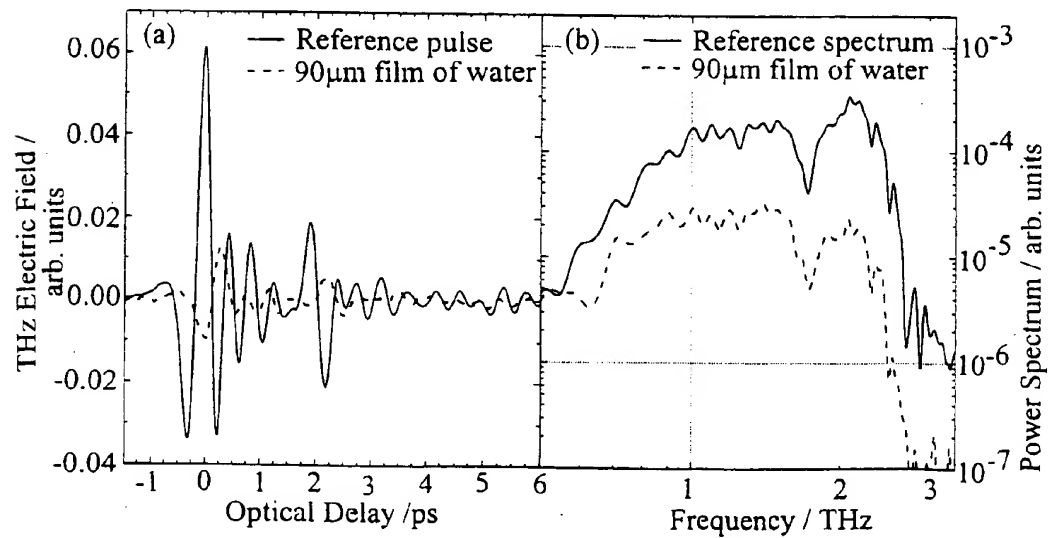


Fig. 12

9/42

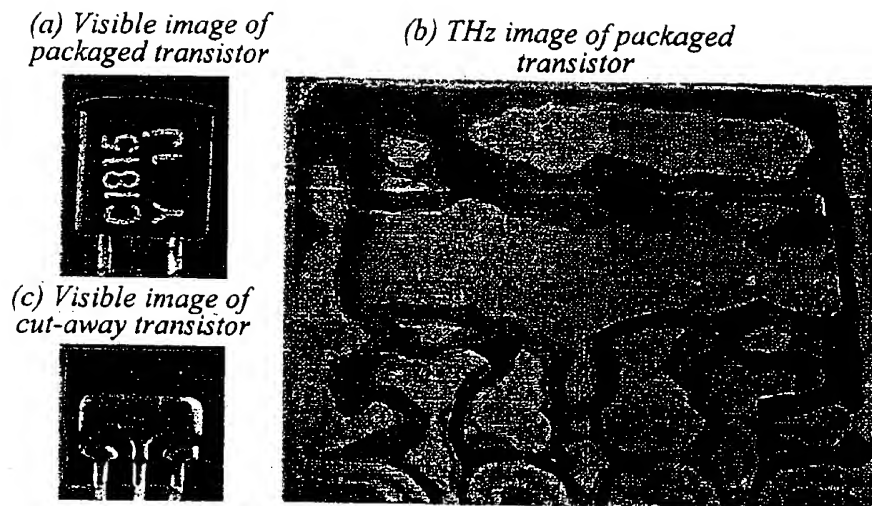


Fig. 13

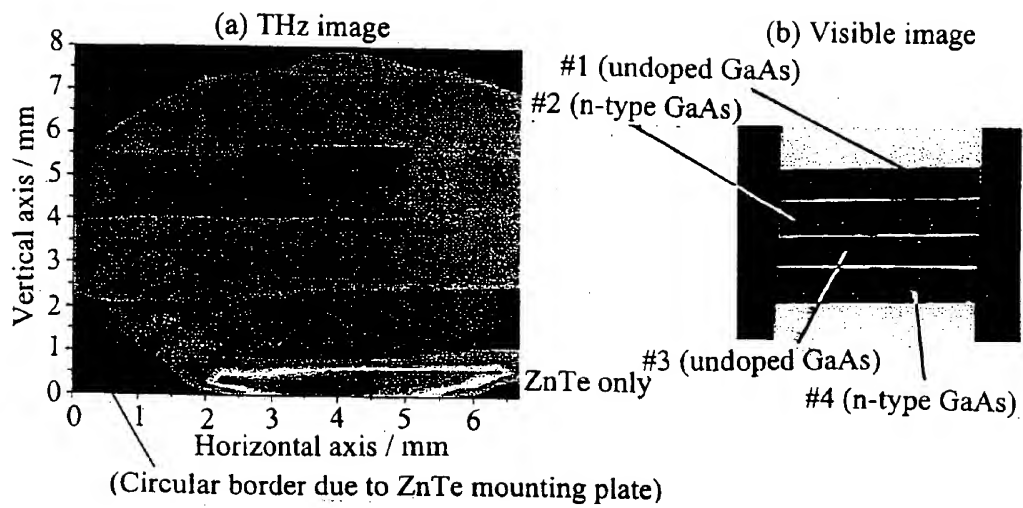


Fig. 14

10/42

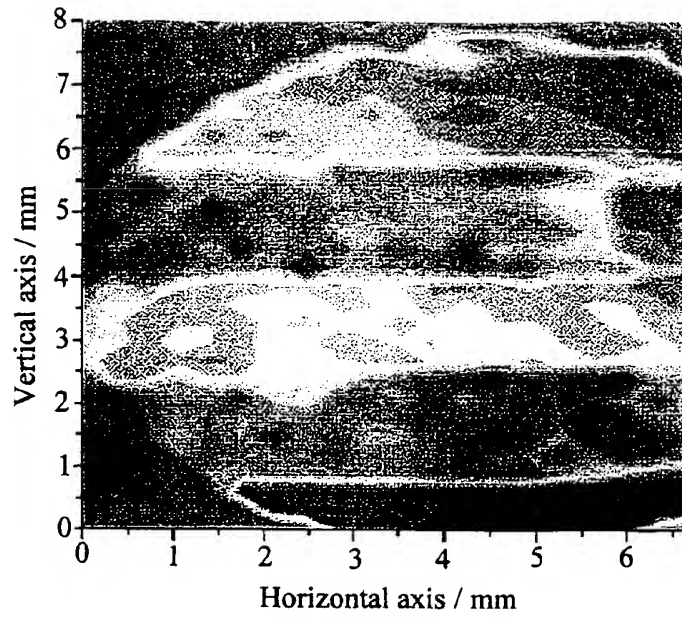


Fig. 15(a)

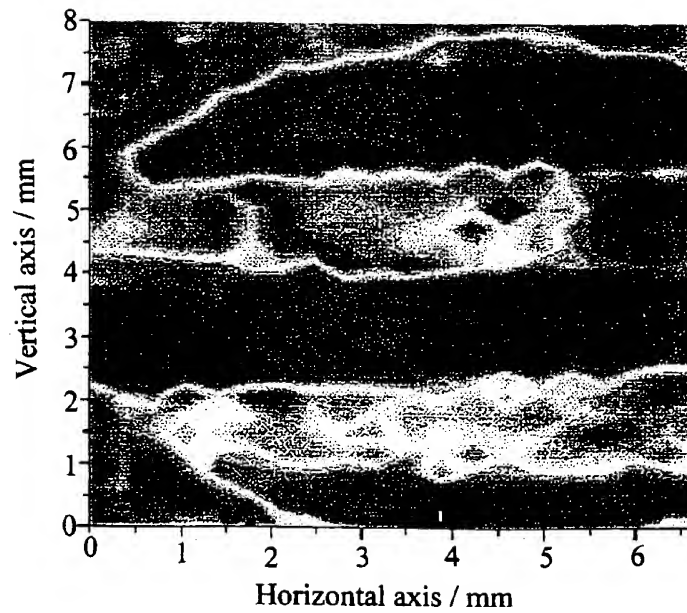


Fig. 15(b)

SUBSTITUTE SHEET (RULE 26)

11/42

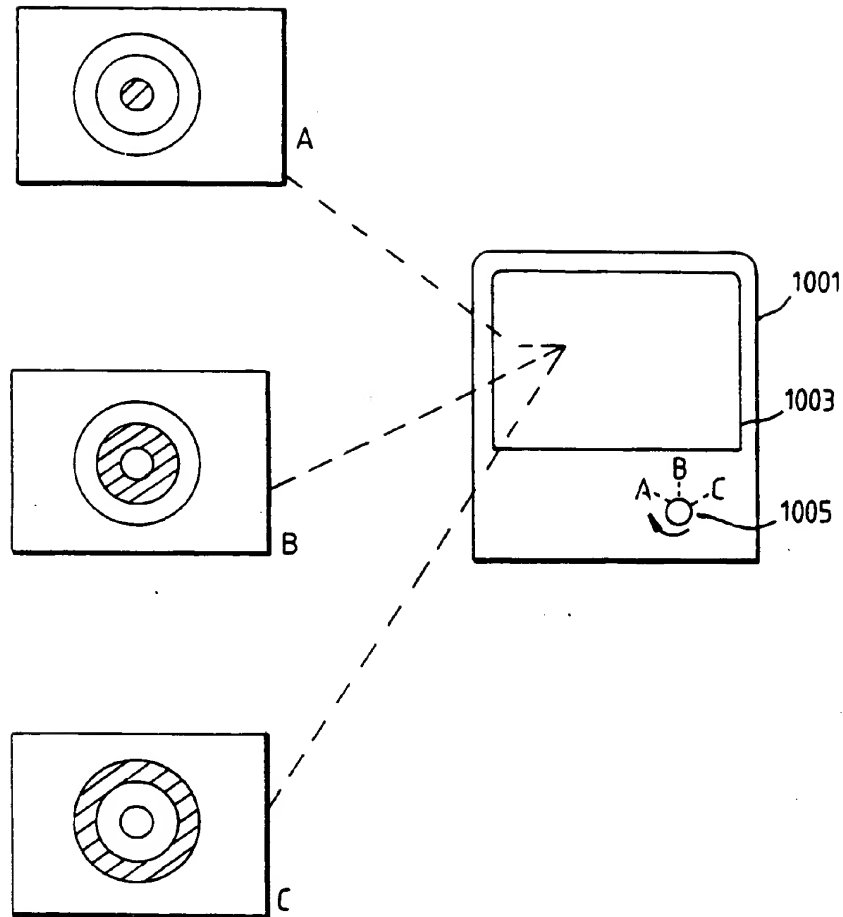


Fig. 16

12/42

fs-ps pulsed visible laser 37

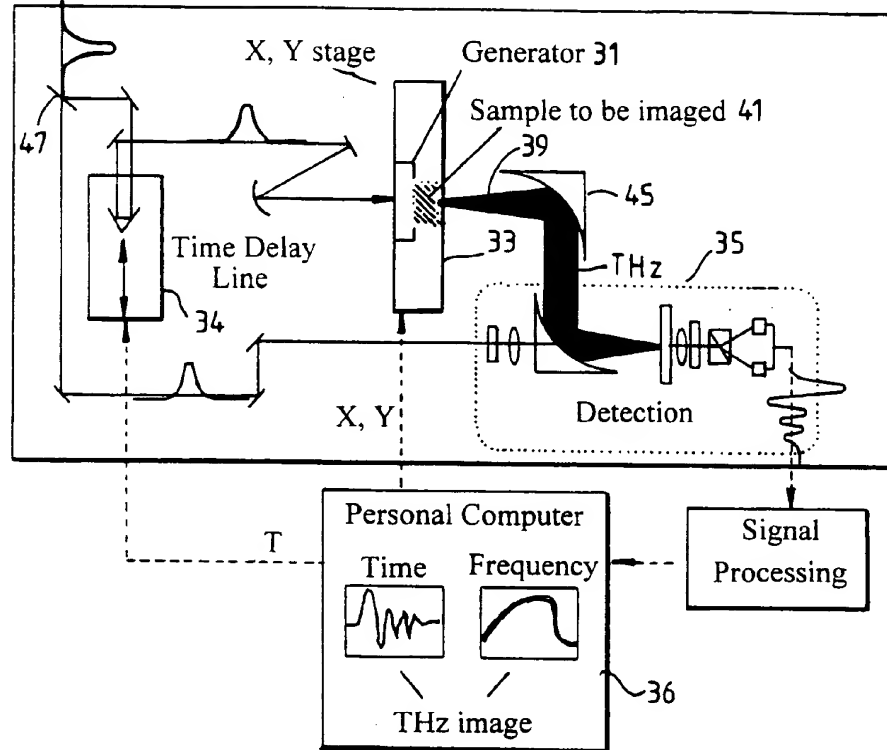
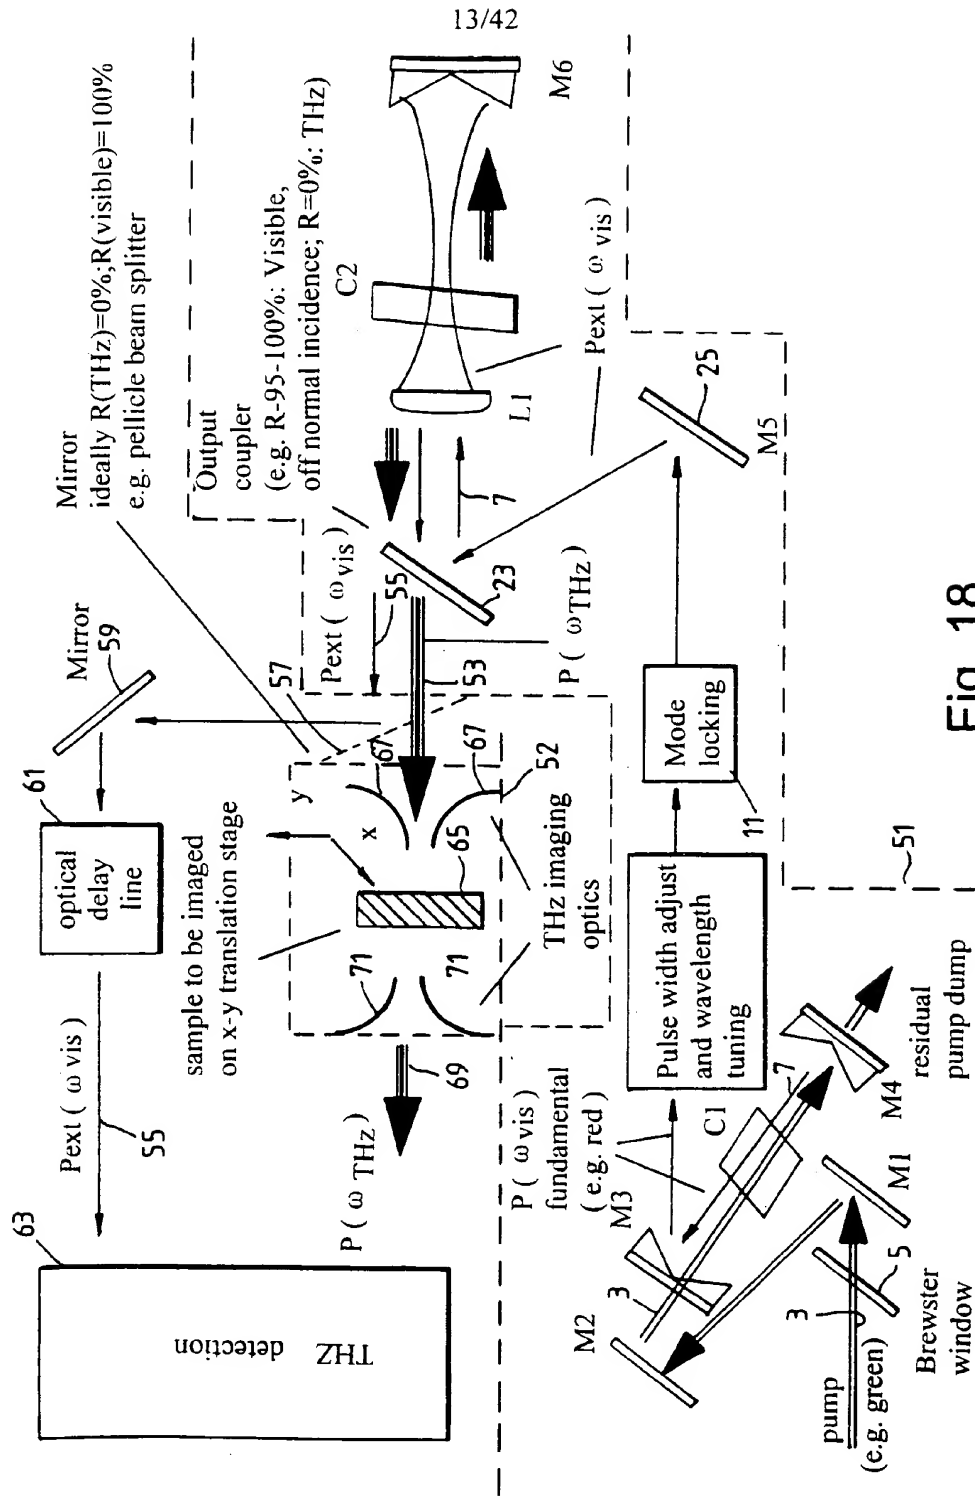
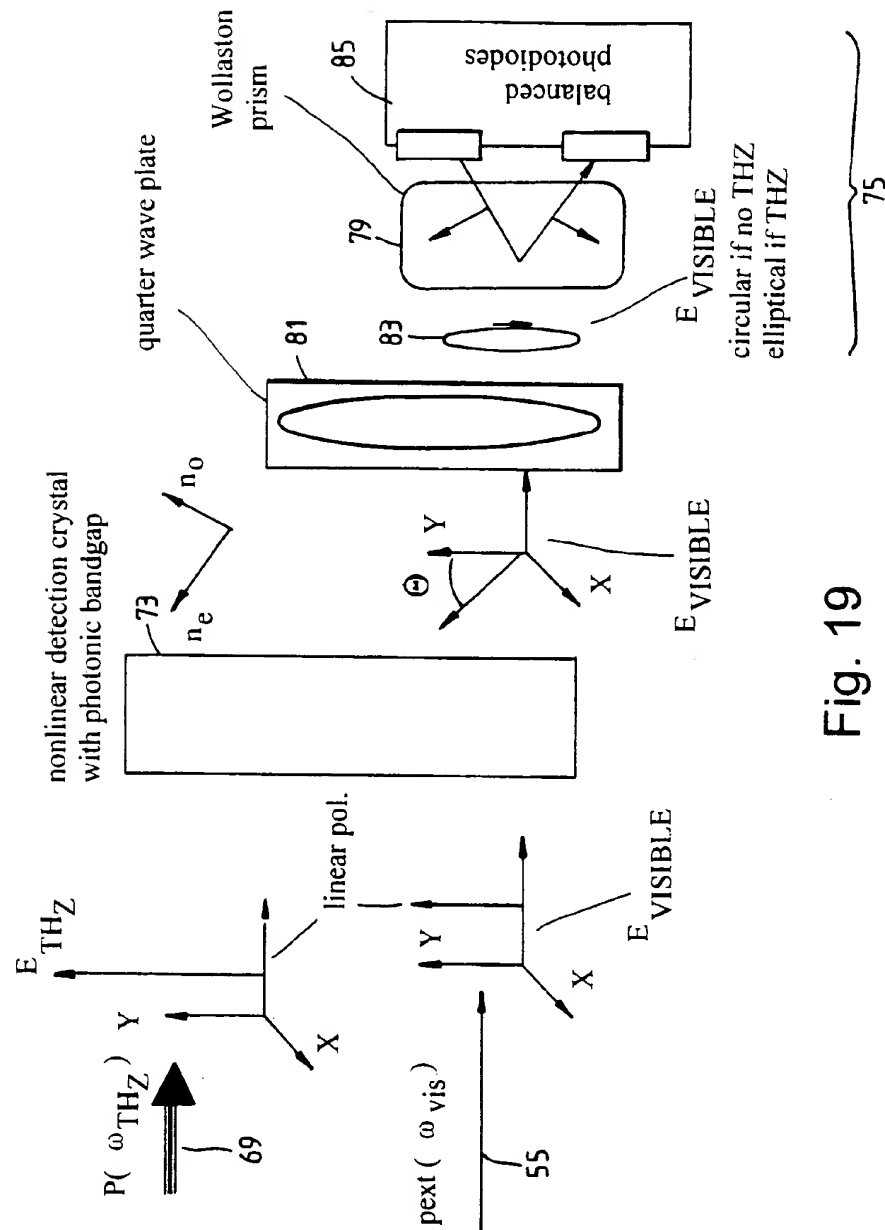
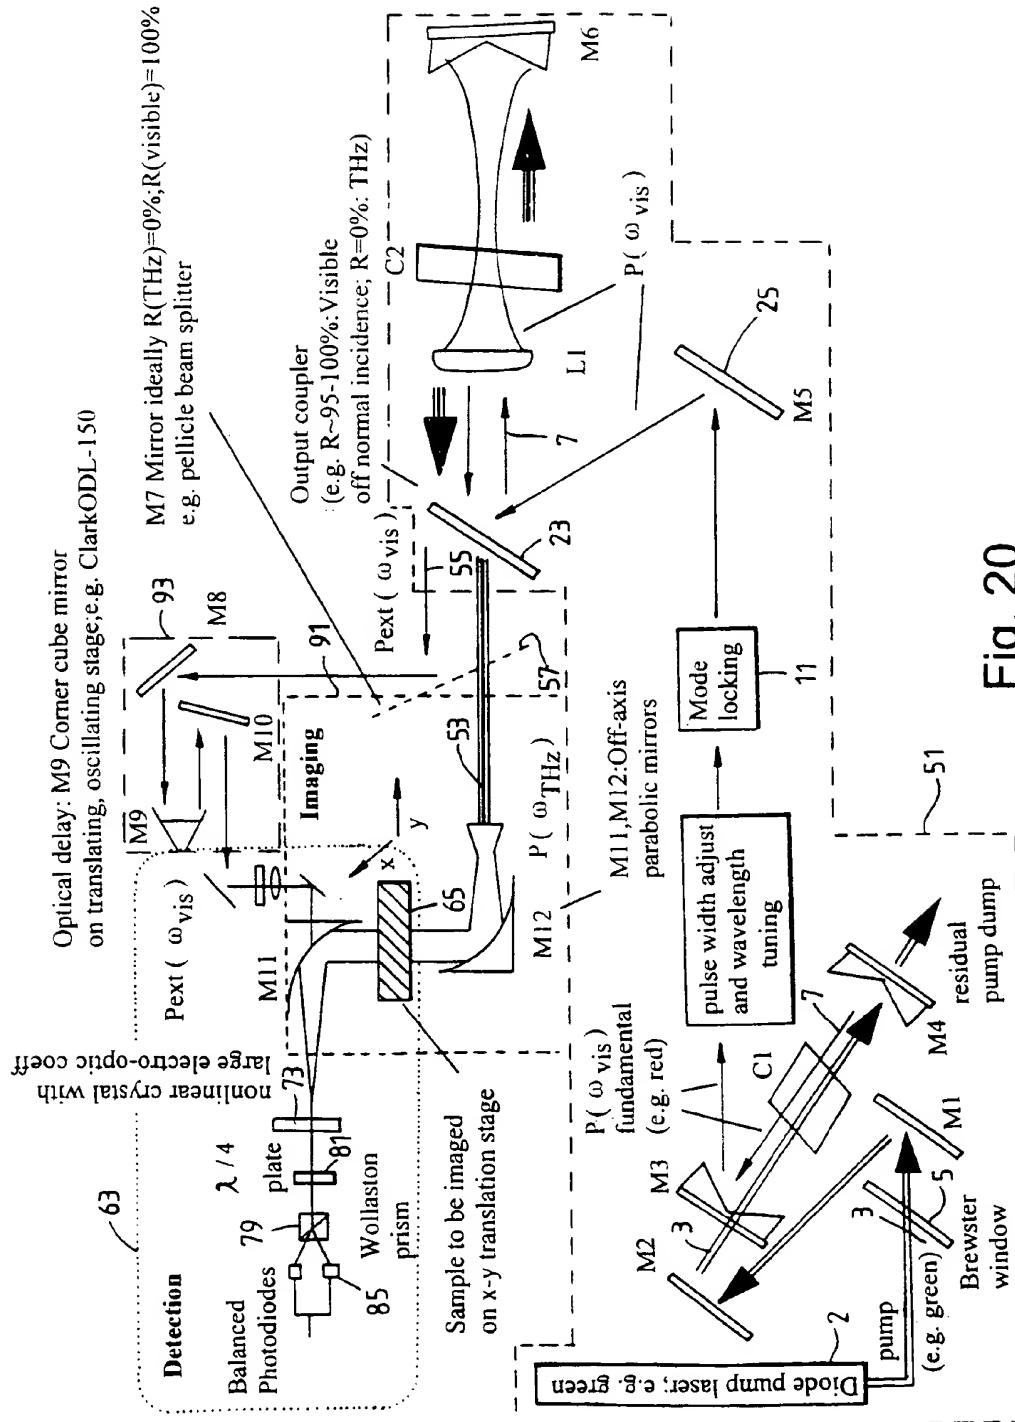


Fig. 17








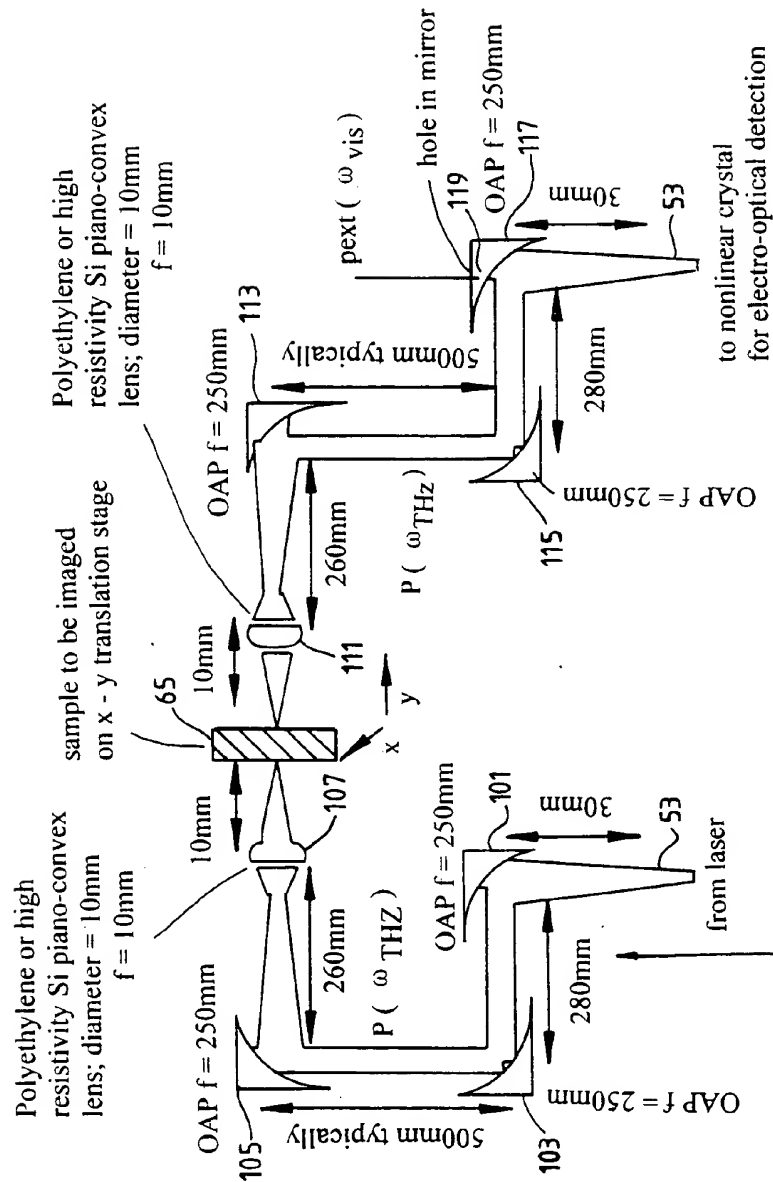


Fig. 21

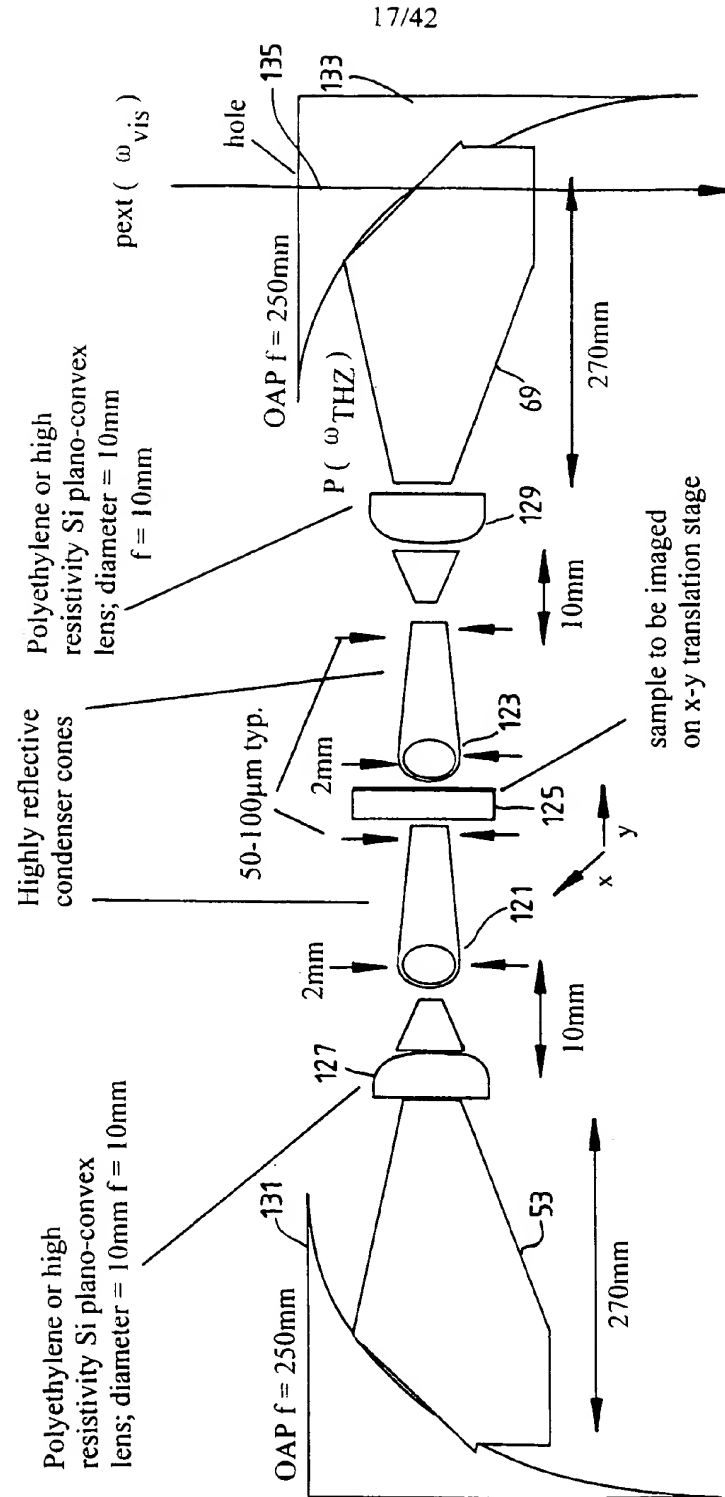

Optional: Lens and condenser cones similar to those in Figure 10 for enhanced spatial resolution in x-y plane of object.

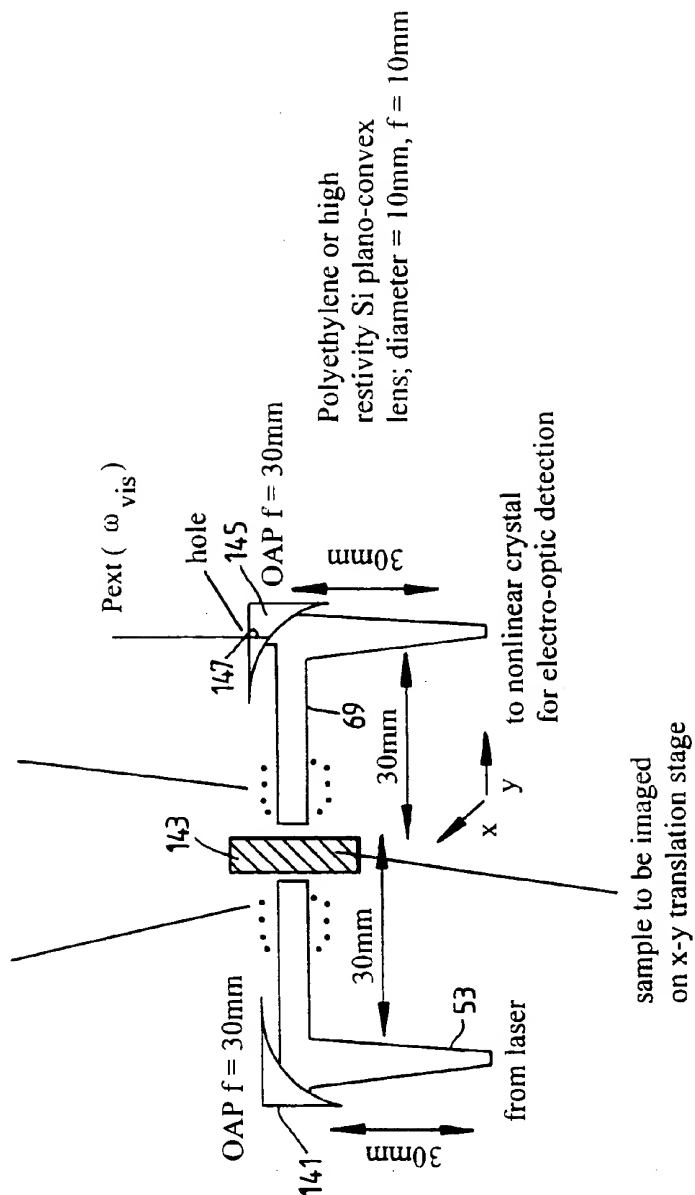


Fig. 23

sample to be imaged
on x-y translation stage

19/42

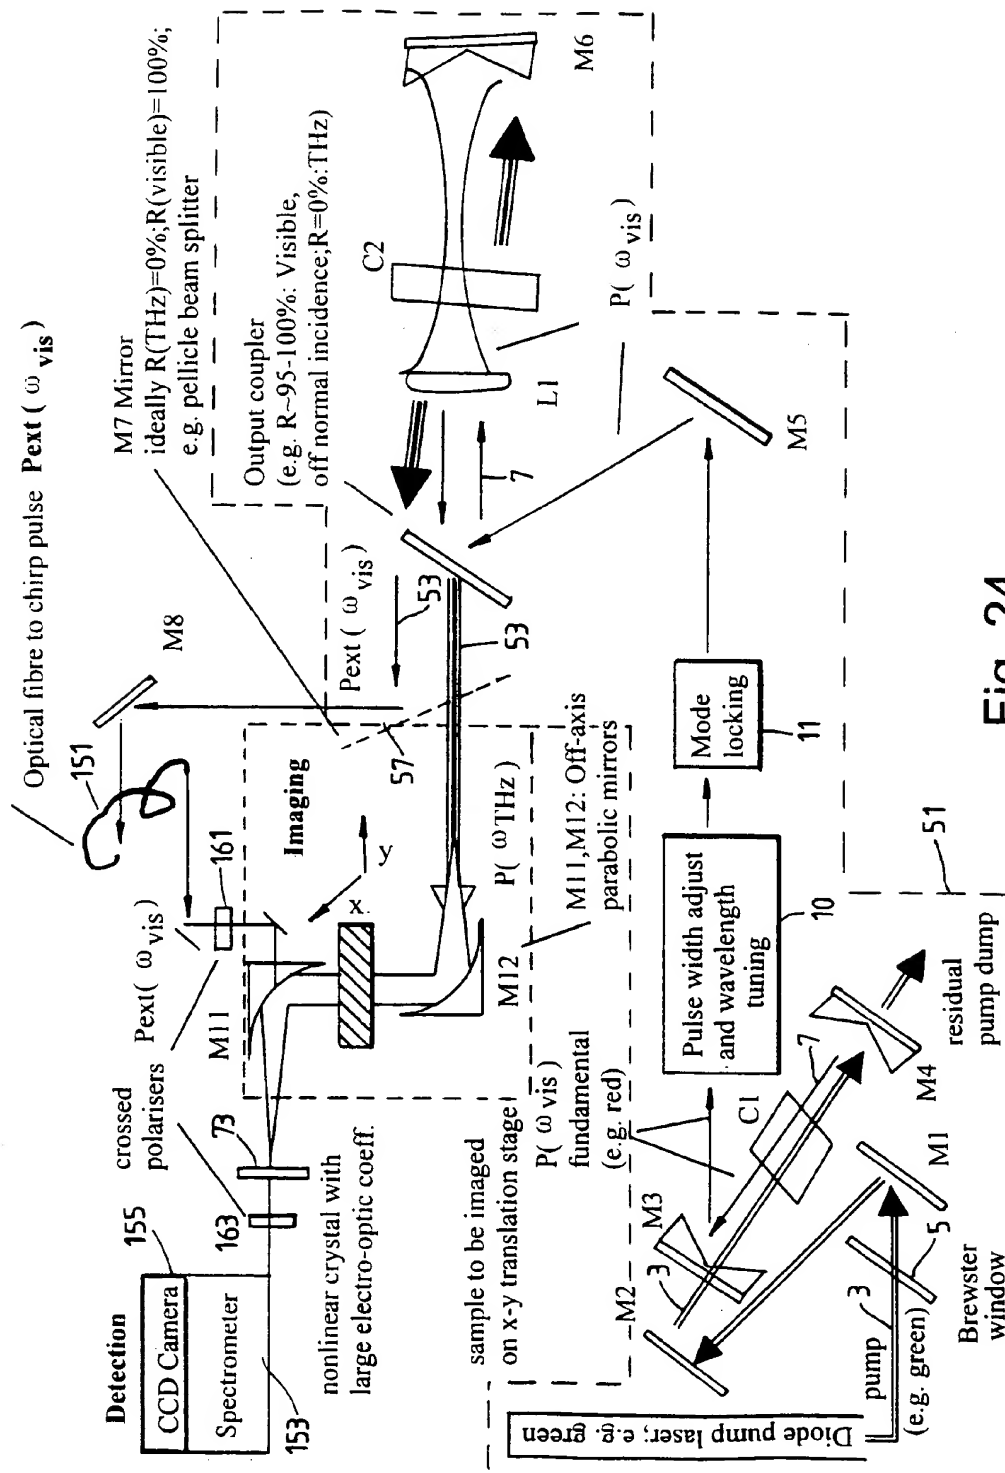


Fig. 24

Fig. 25

21/42

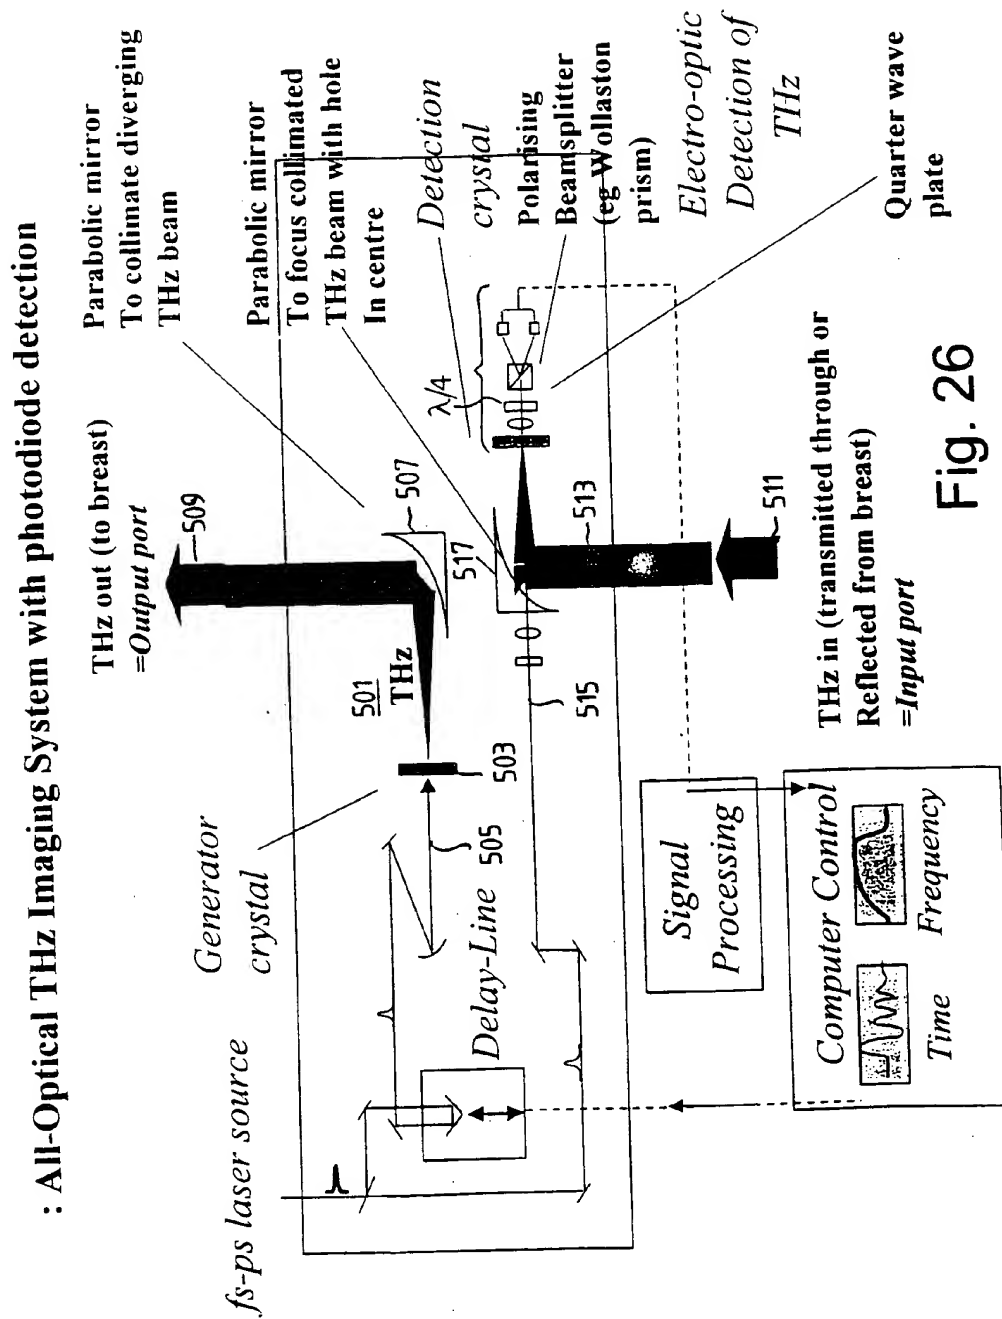


Fig. 26

22/42

: All-Optical THz Imaging System with CCD detection

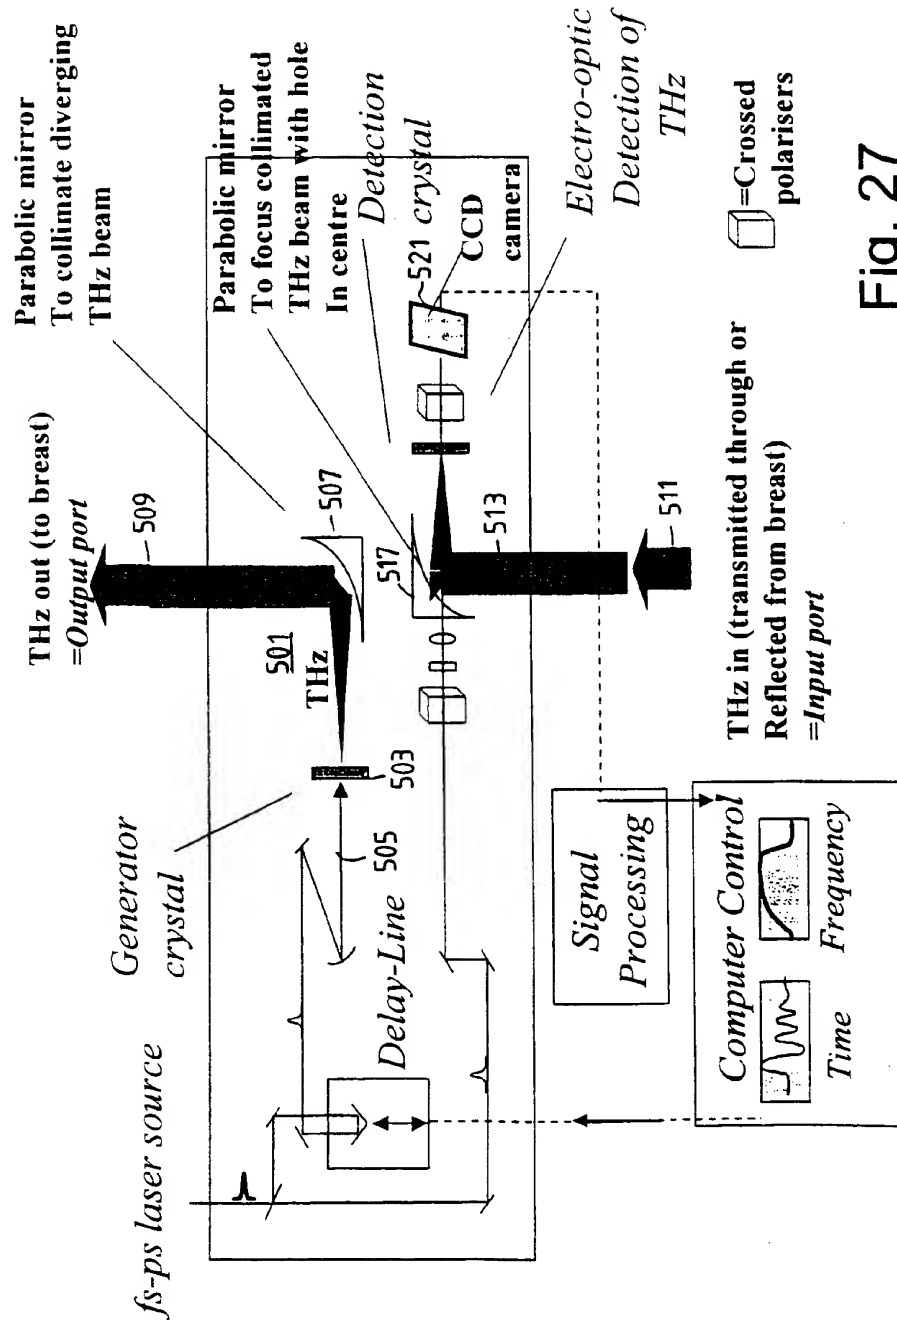


Fig. 27

: Sample port for THz breast screening
(for use with all-optical systems in Figures 2 and 3)



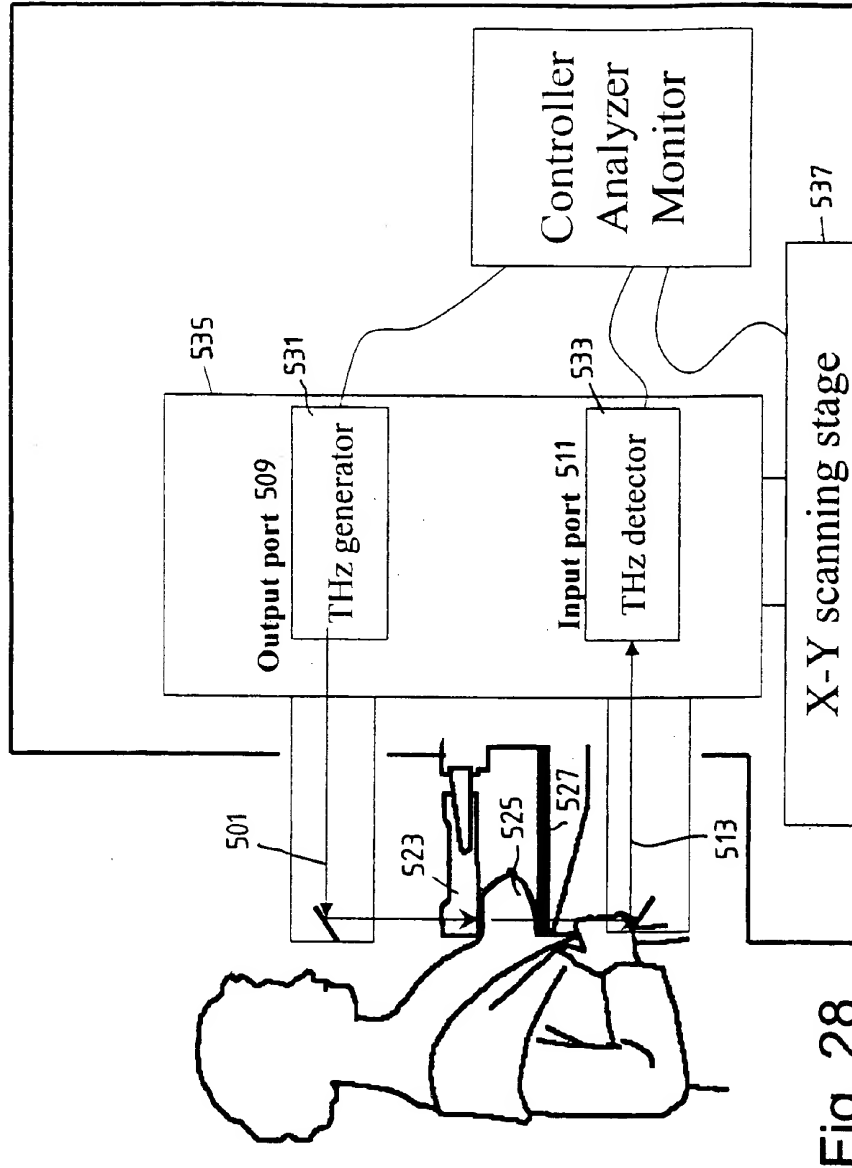


Fig. 28

: Sample port for THz breast screening
(for use with all-optical systems in Figures 2 and 3)

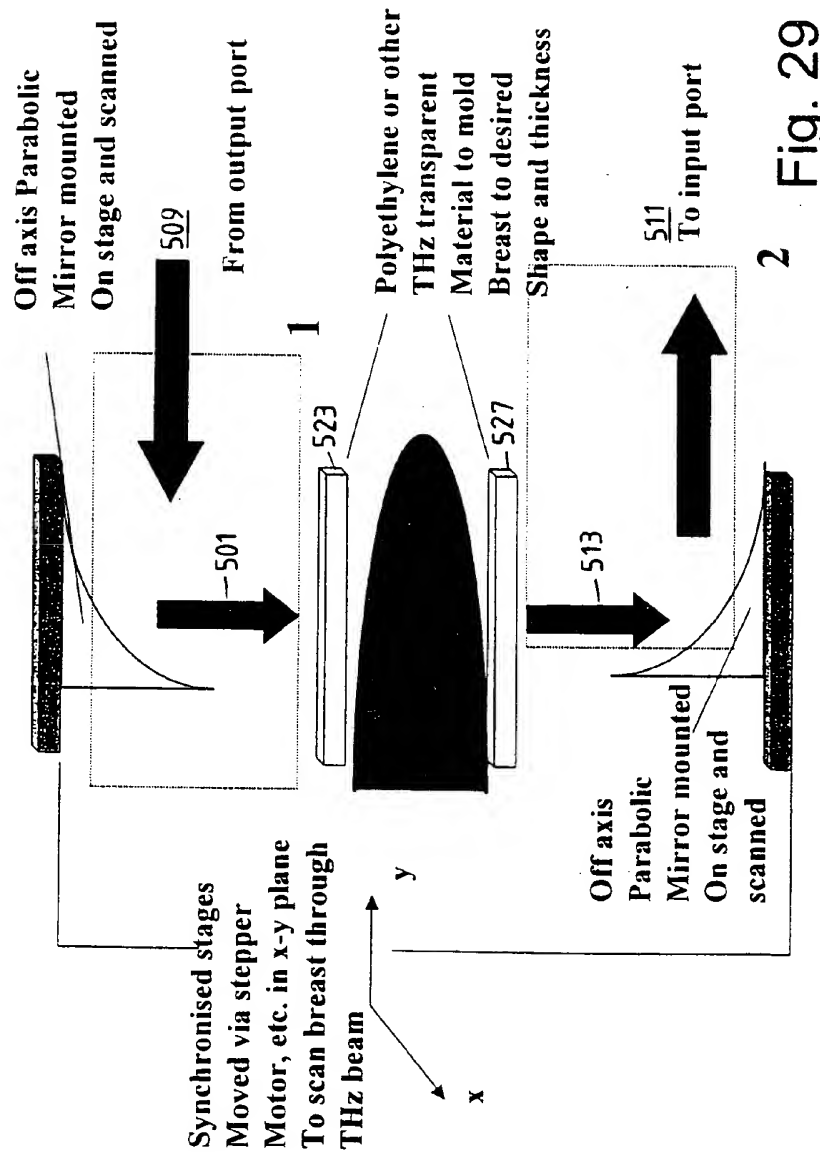

: Possible alternative configuration of coupling optics
used in Figure 5 (regions denoted 1. And 2. In dotted boxes).

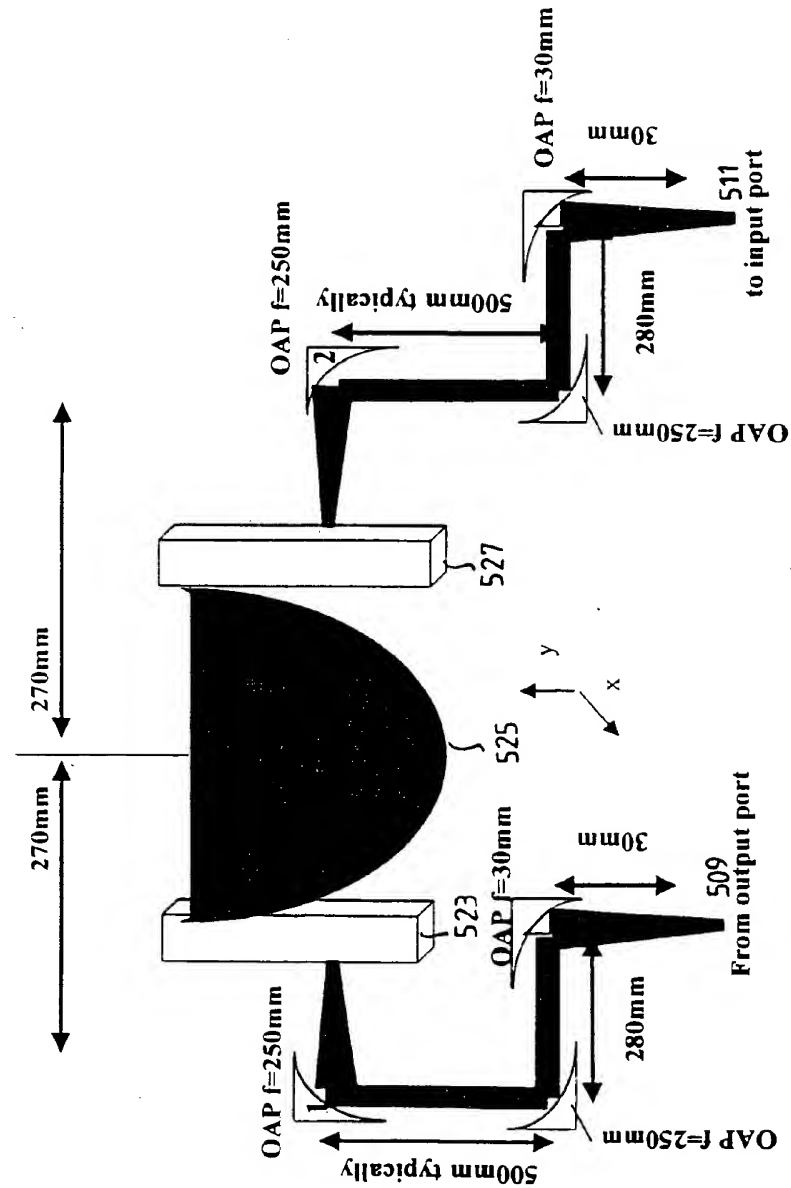

All mirrors are off-axis parabolics (OAPs).
OAP's designated by 1. And 2. Are on synchronised
X-Y stepper motor stages

Fig. 31

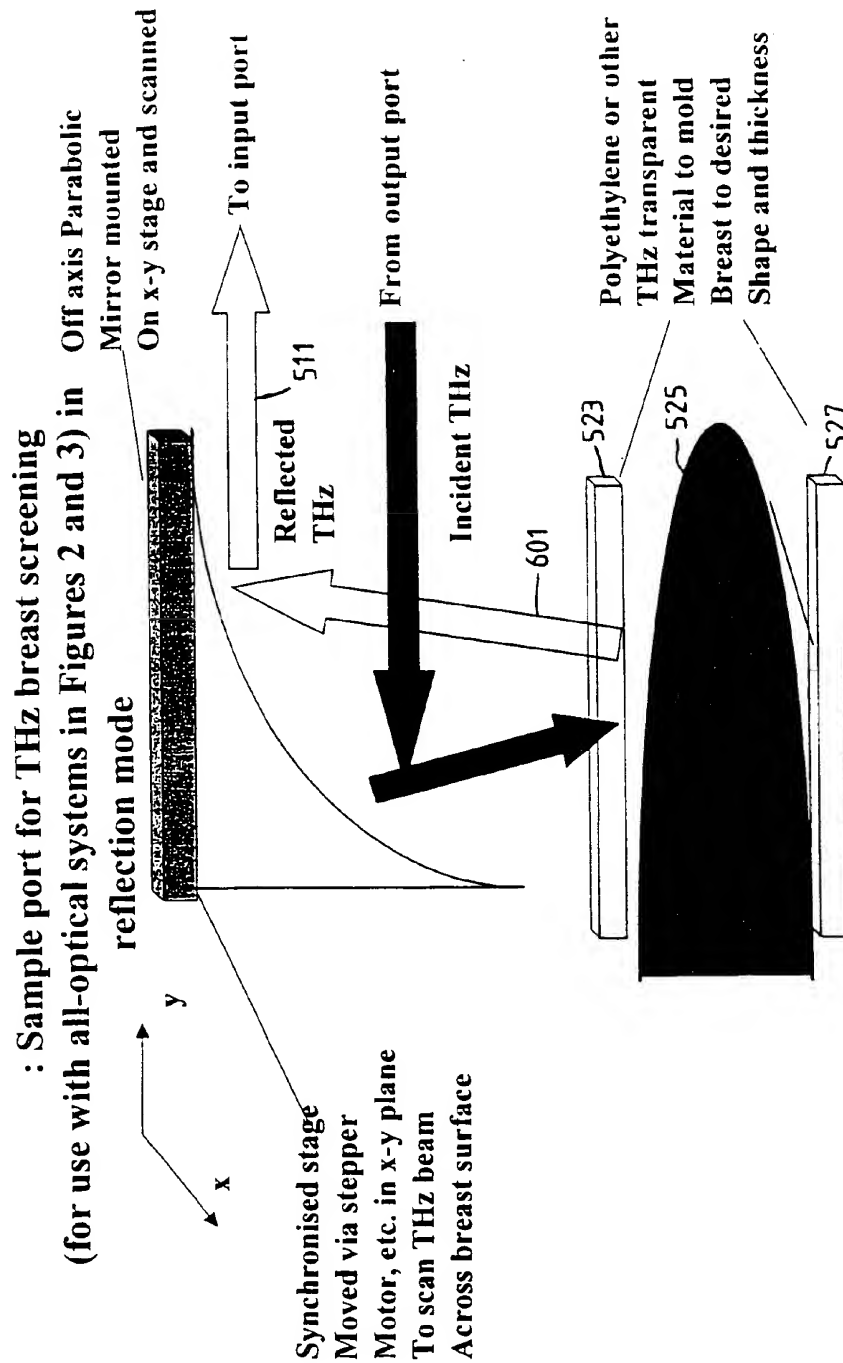


Fig. 32

All mirrors are off-axis parabolics (OAPs).

28/42

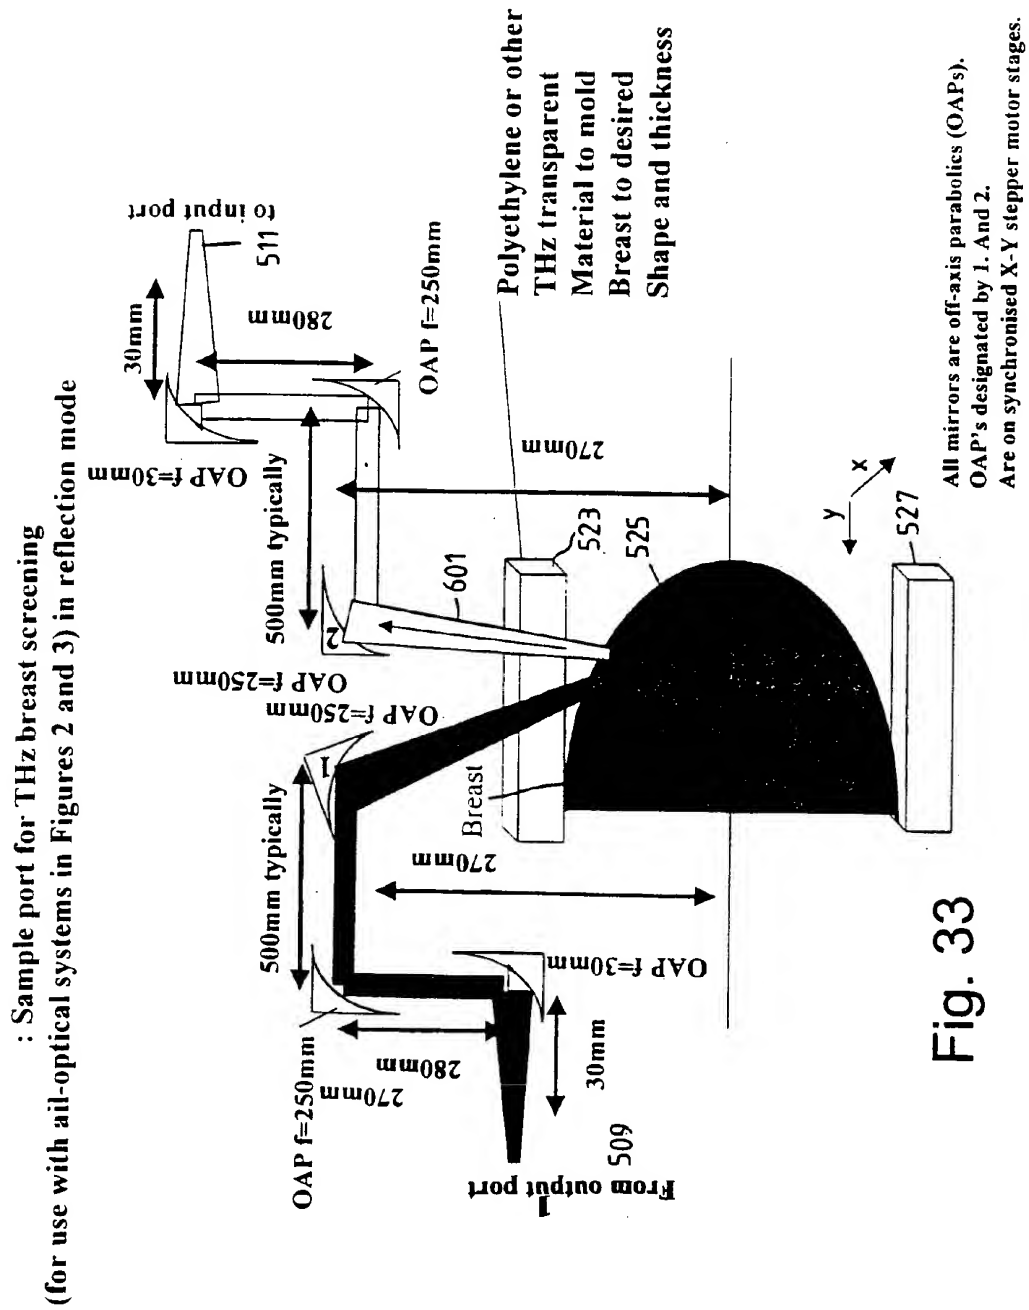


Fig. 33

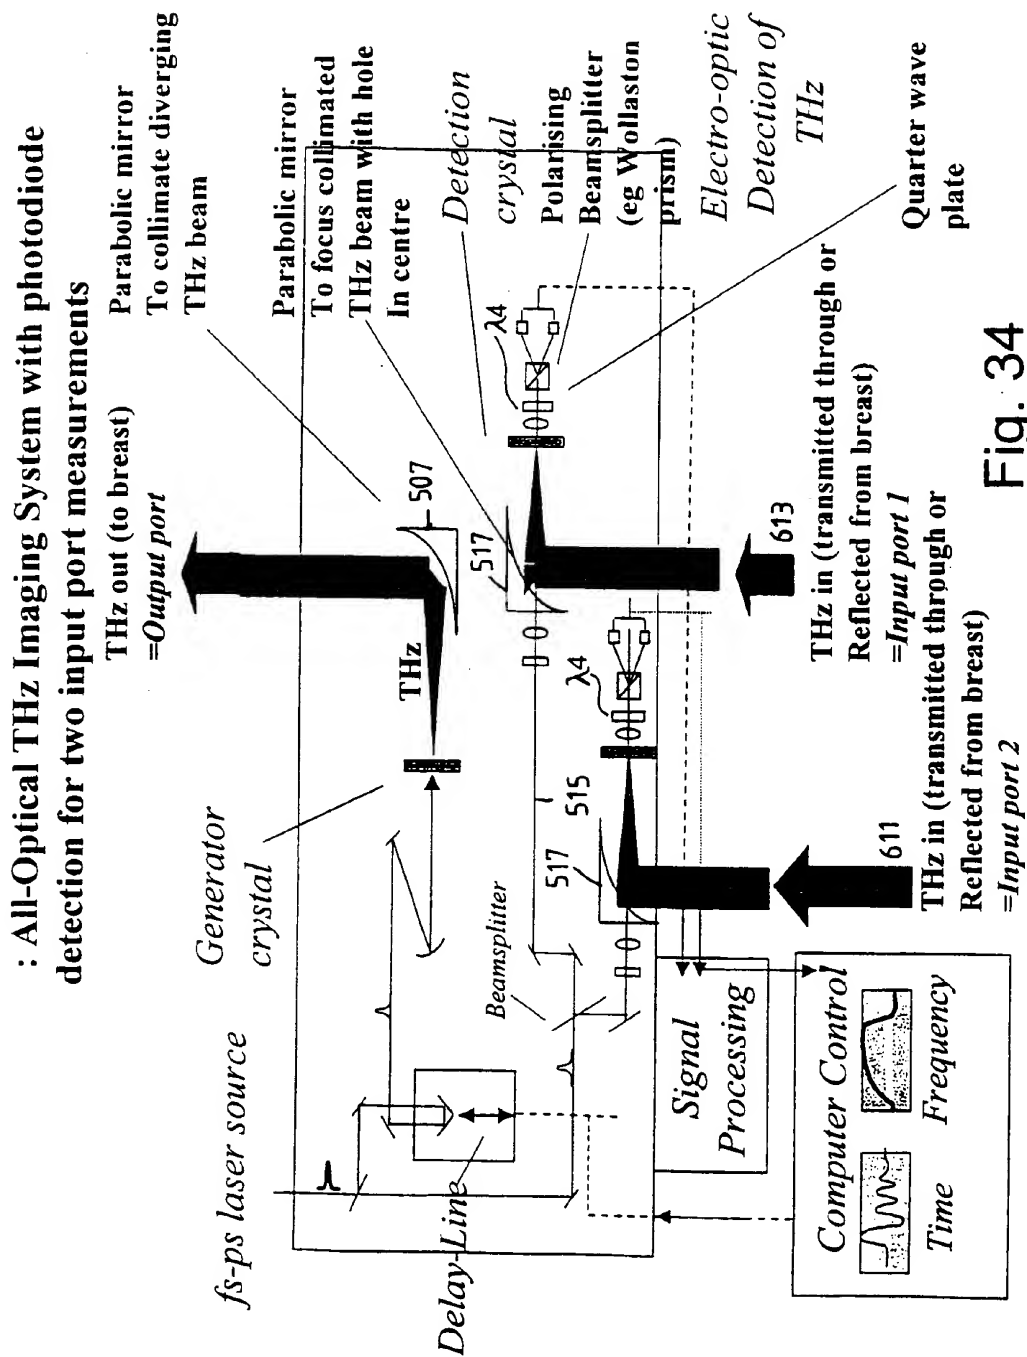


Fig. 34

**: All-Optical THz Imaging System with photodiode
detection for two input port measurements**



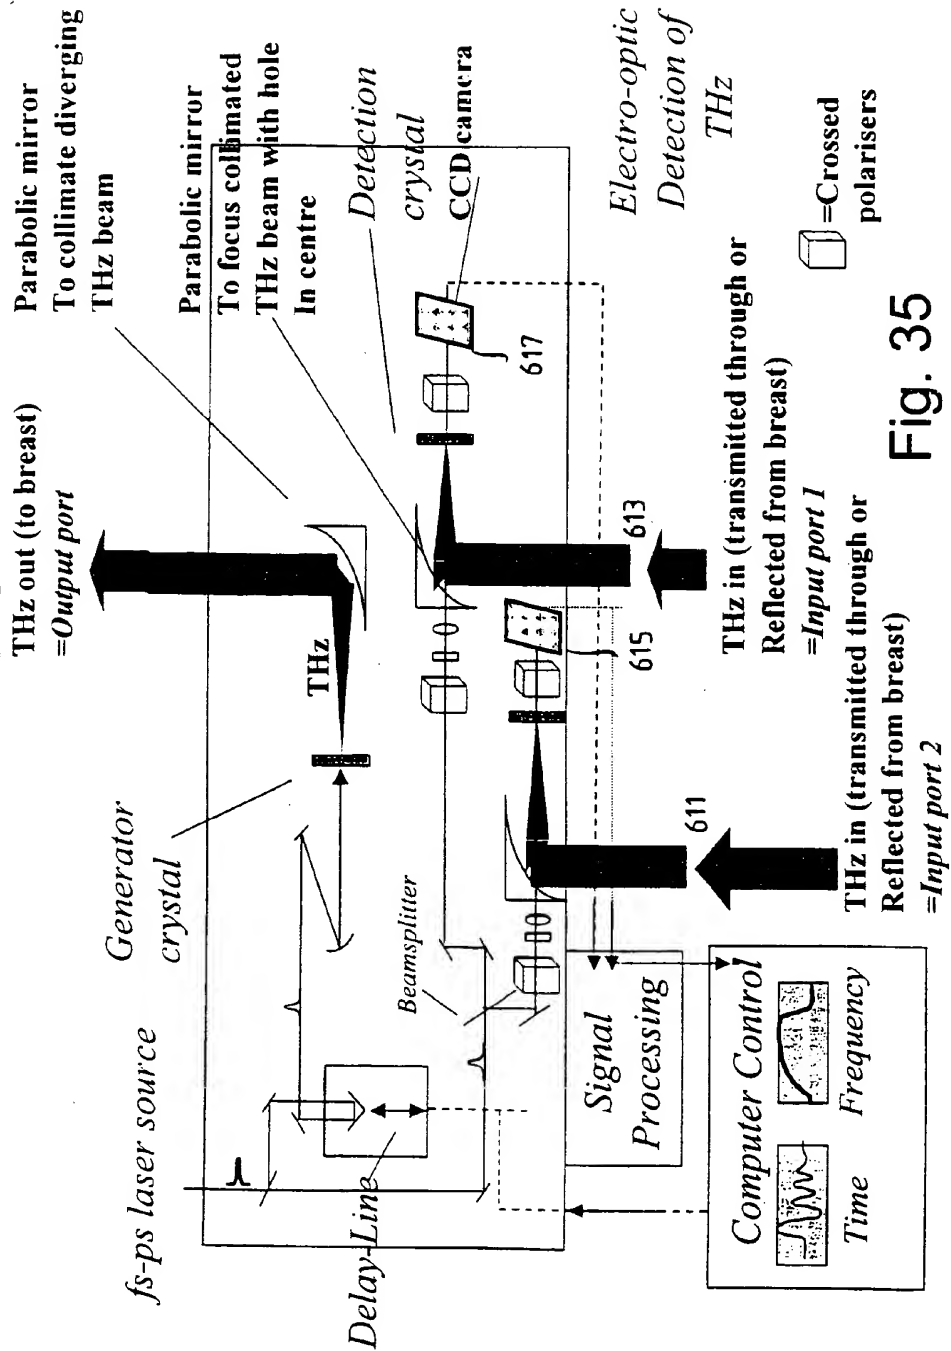


Fig. 35

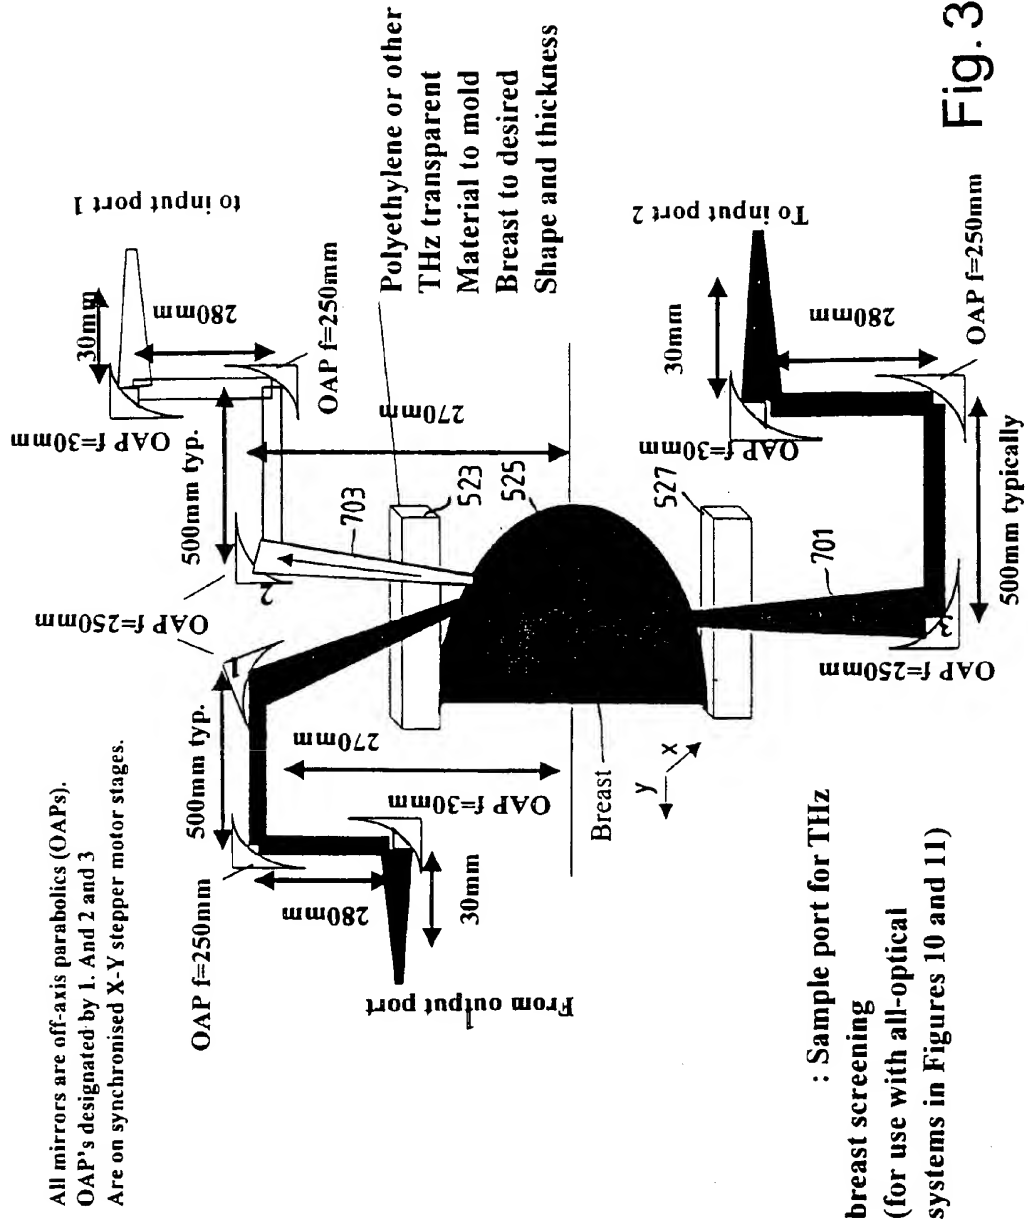


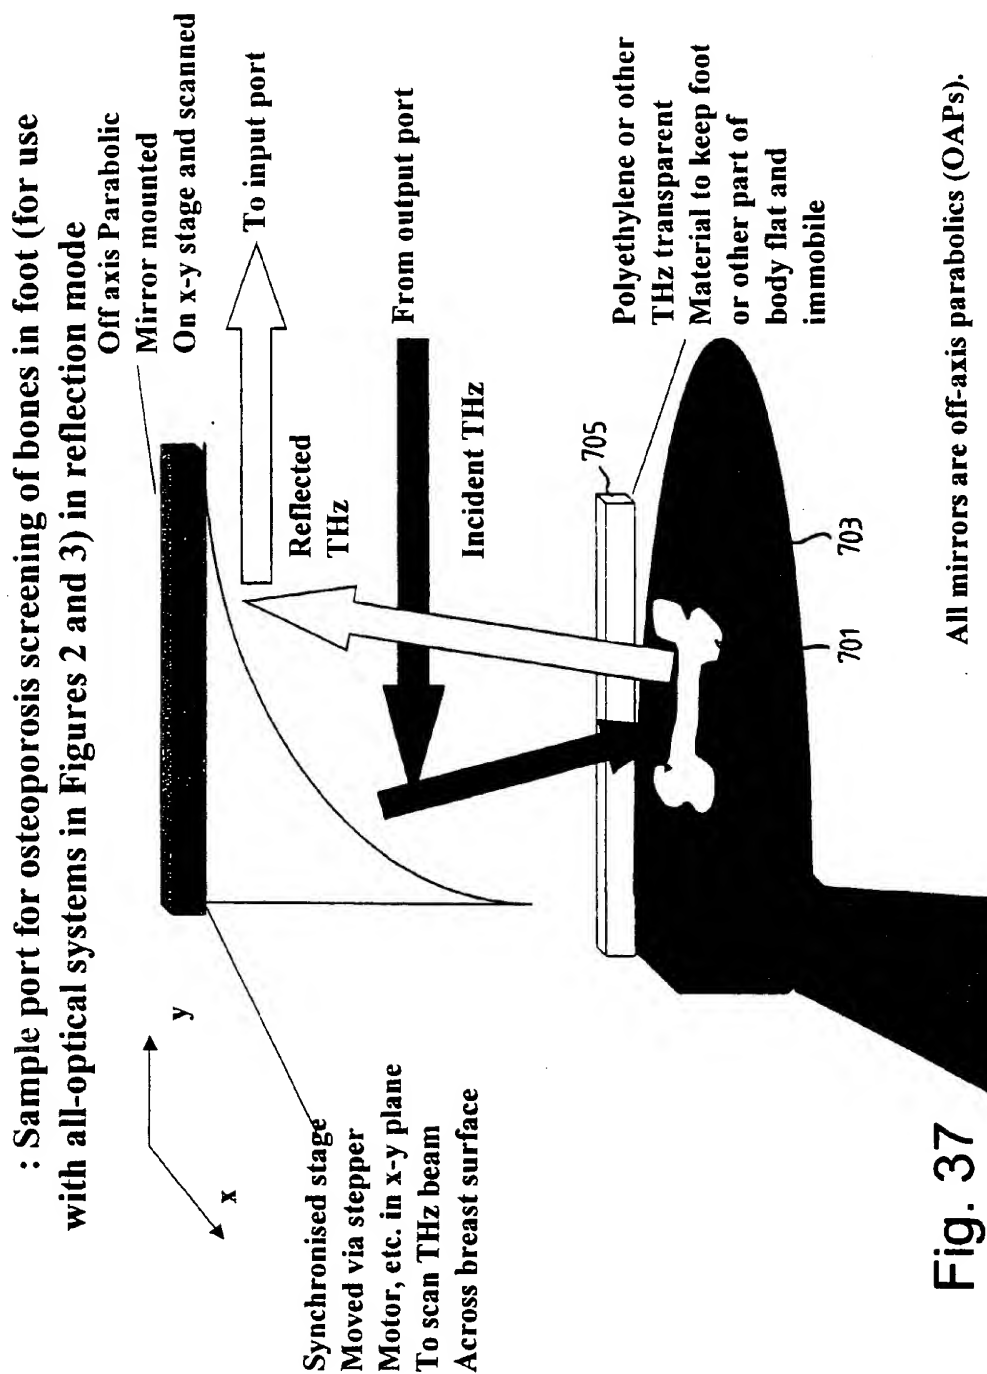

33/42


: THz transmission through animal bone

Example of 2 bones - visible image

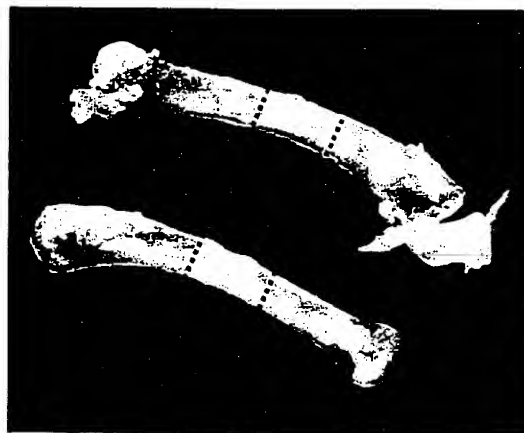

(a)

3D THz image through 2 bone sample

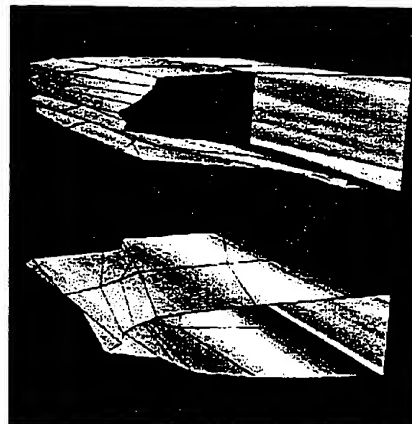

(b)

Fig. 38

: Medical Imaging using Terahertz light in a human tooth

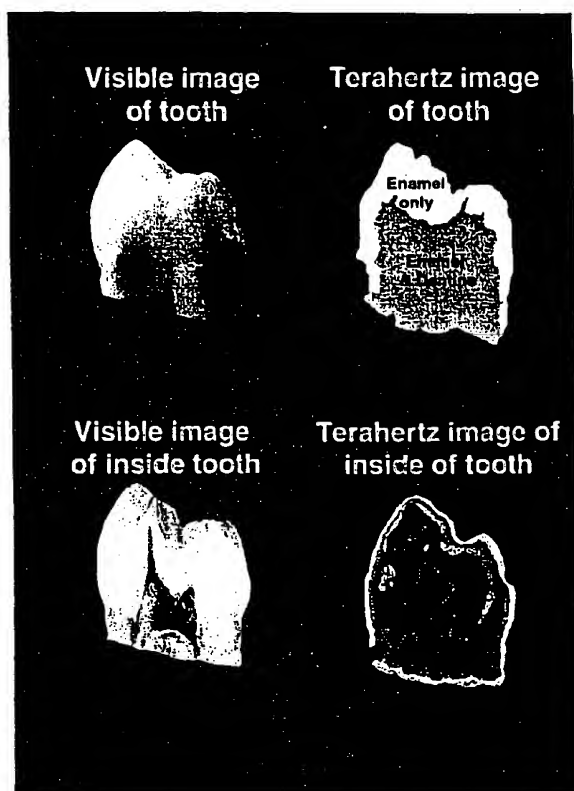


Fig. 39

: THz imaging of different types of animal tissue: clotted blood

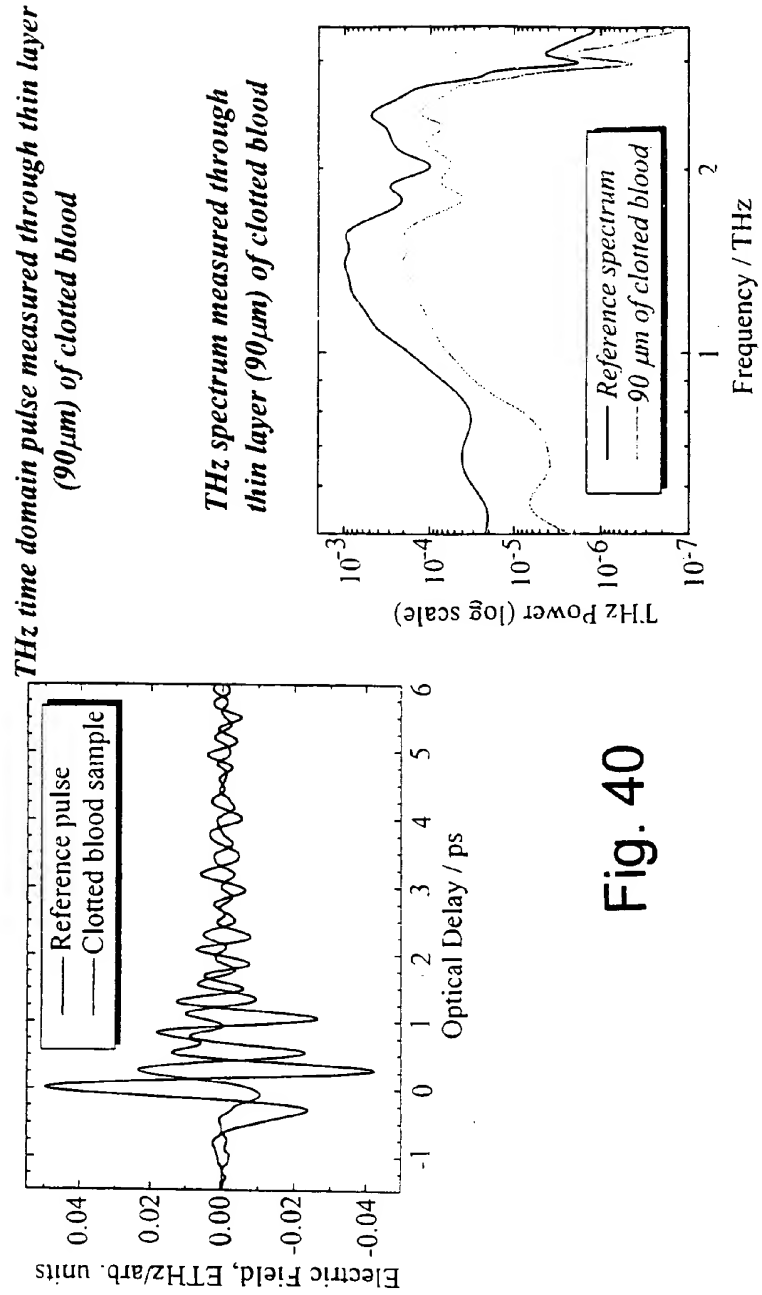


Fig. 40

36/42

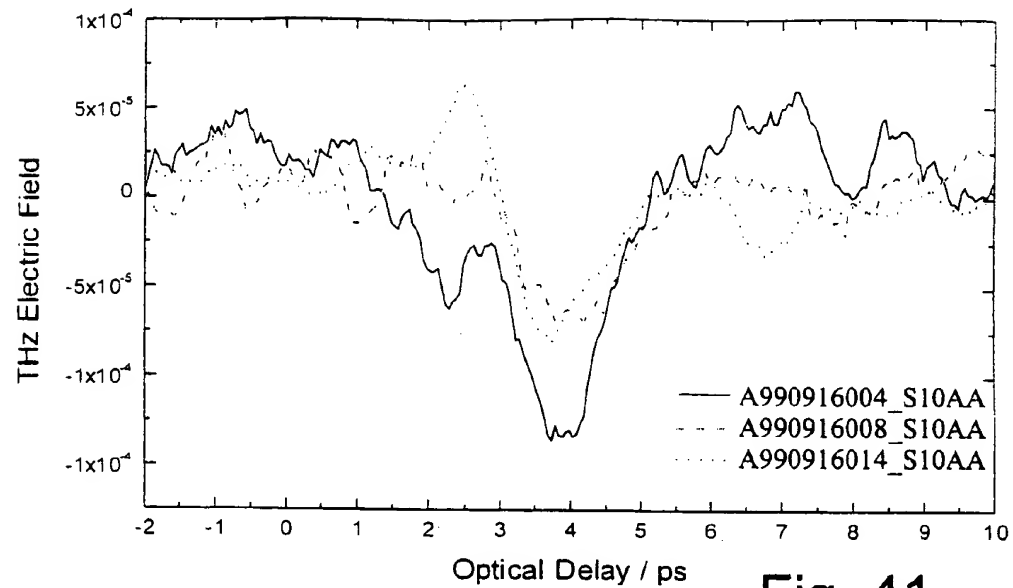


Fig. 41

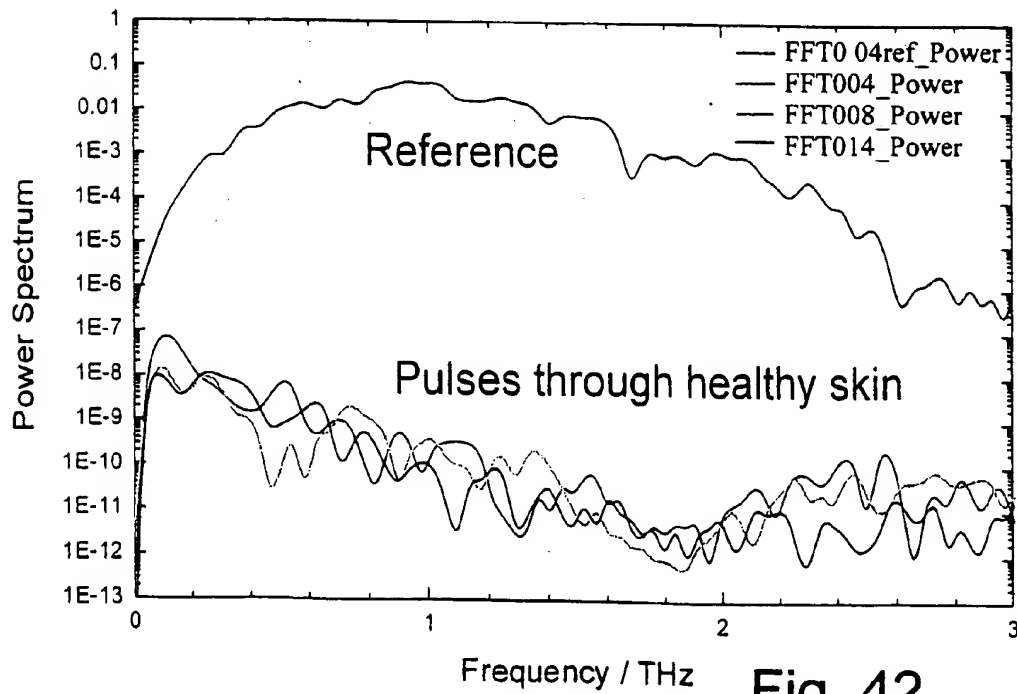


Fig. 42

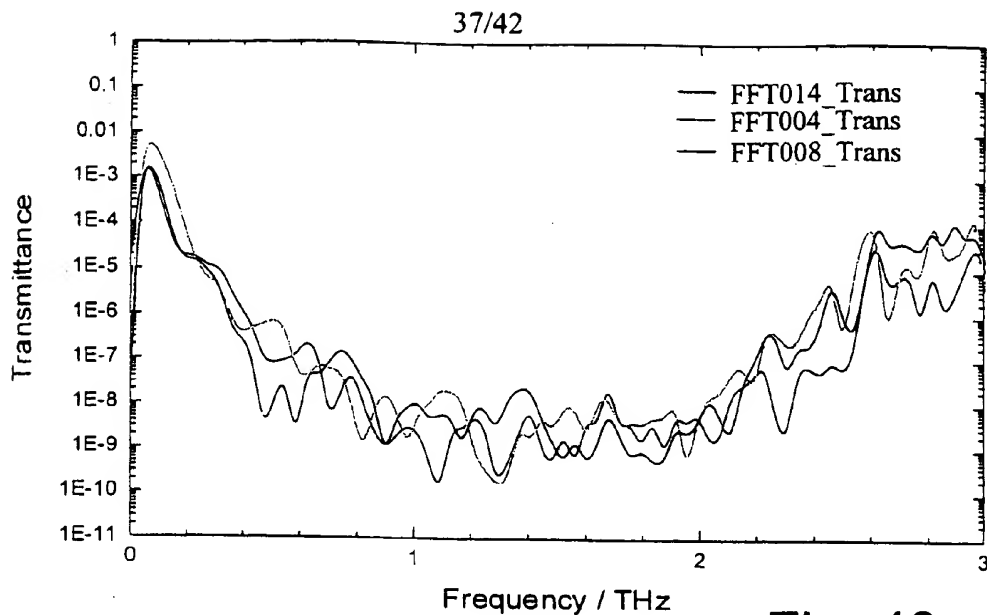


Fig. 43

Transmittance = (signal through skin)/(reference signal)

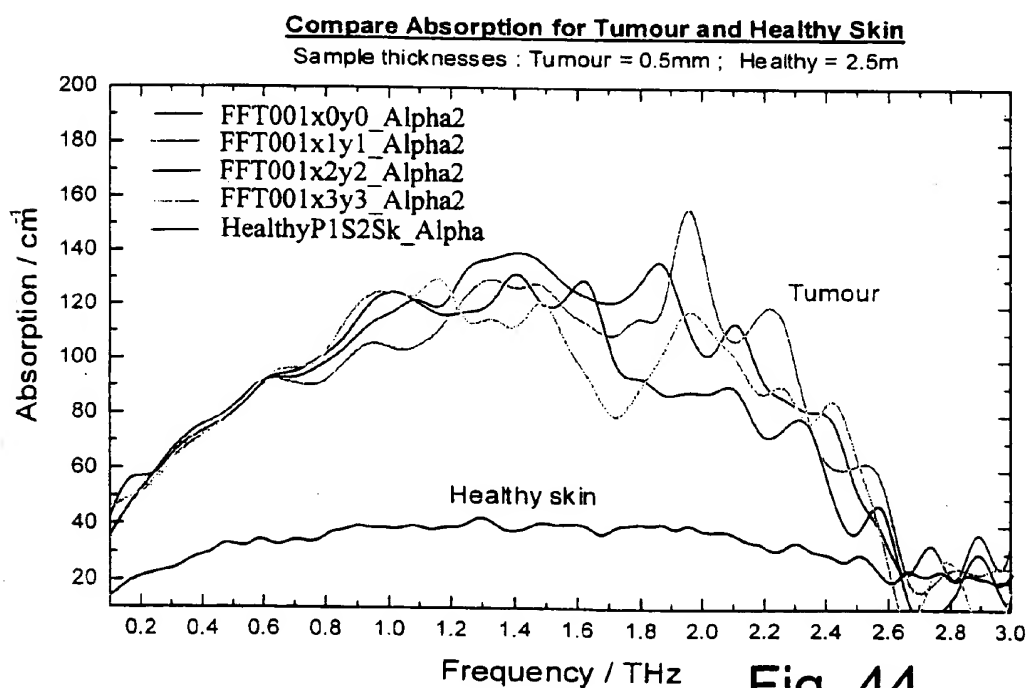


Fig. 44

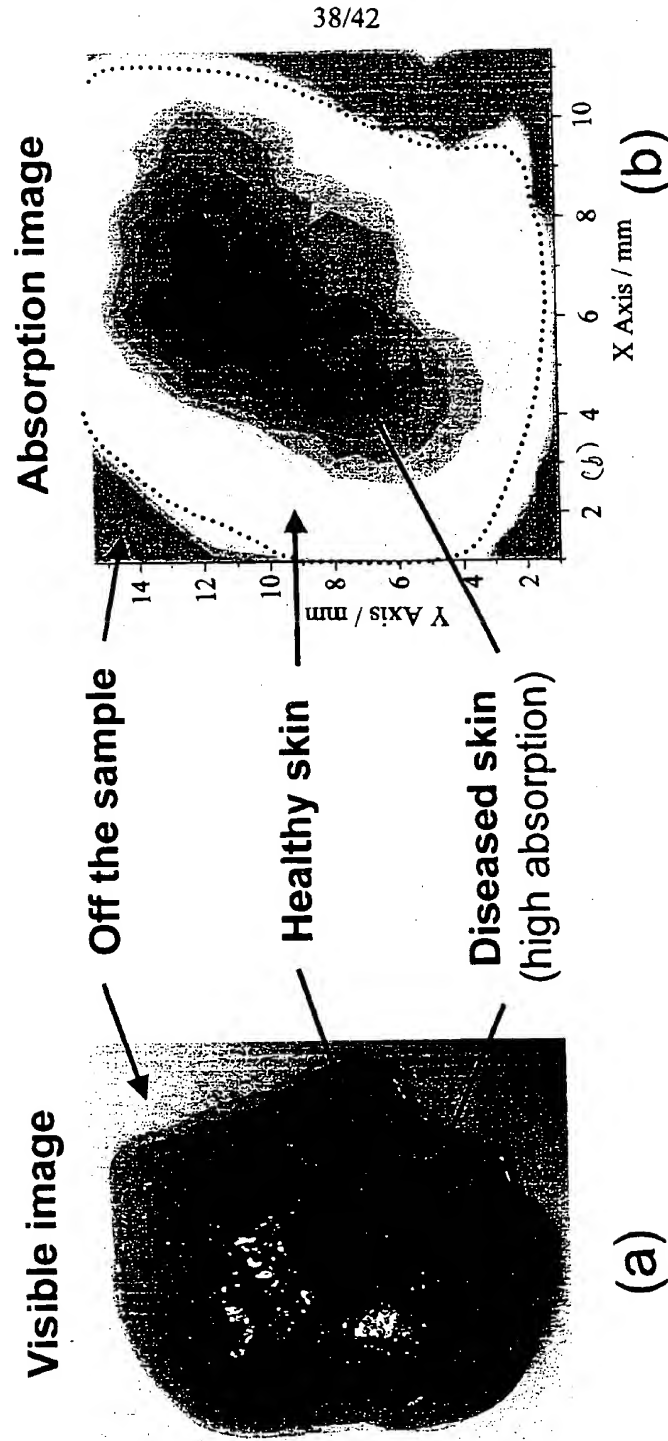


Fig. 45 THz Pulse Laboratory

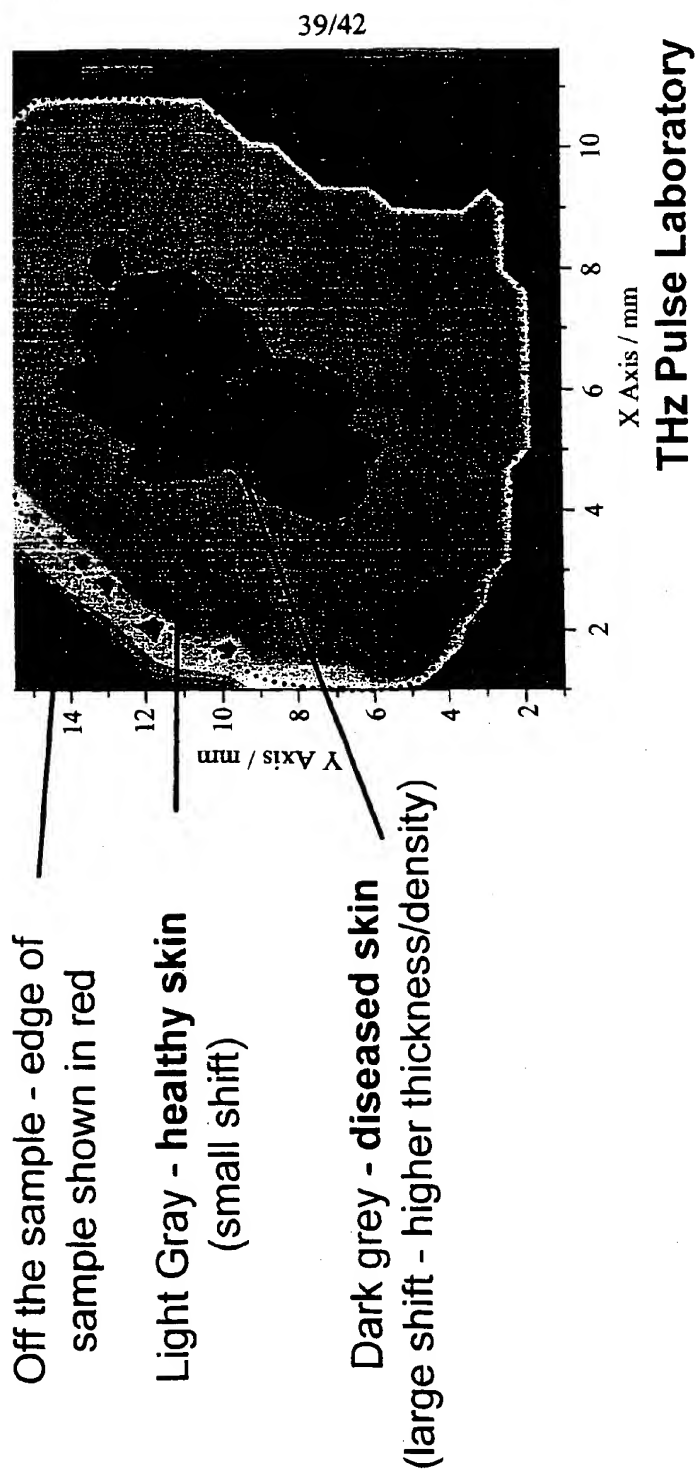


Fig. 46

40/42

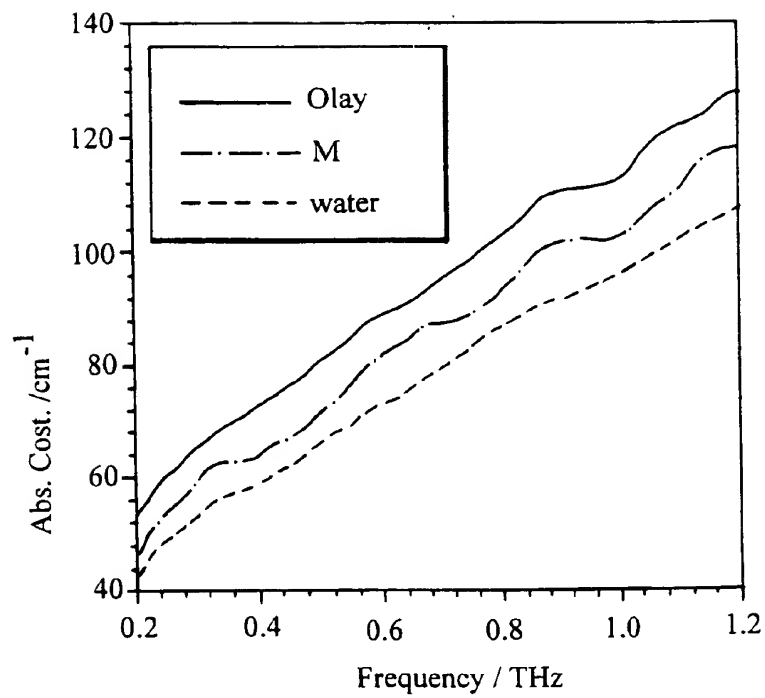


Fig. 47

41/42

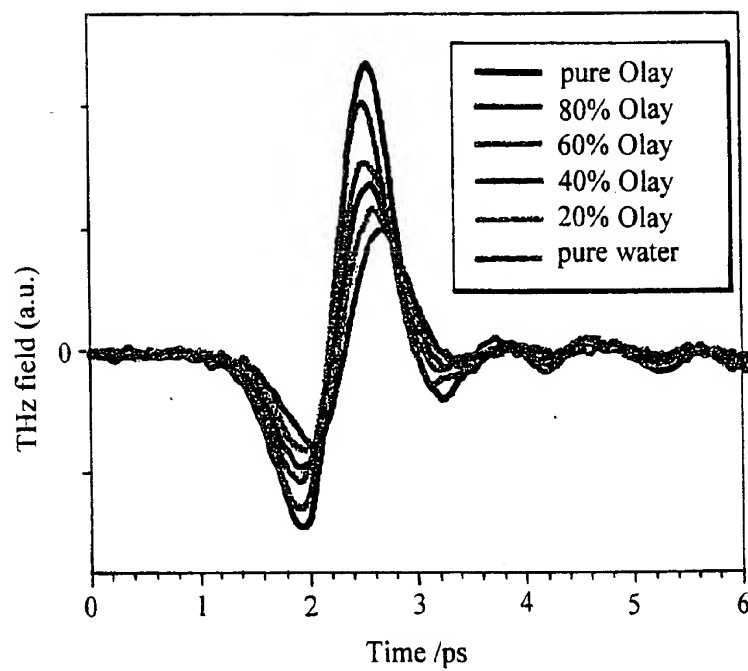


Fig. 48

42/42

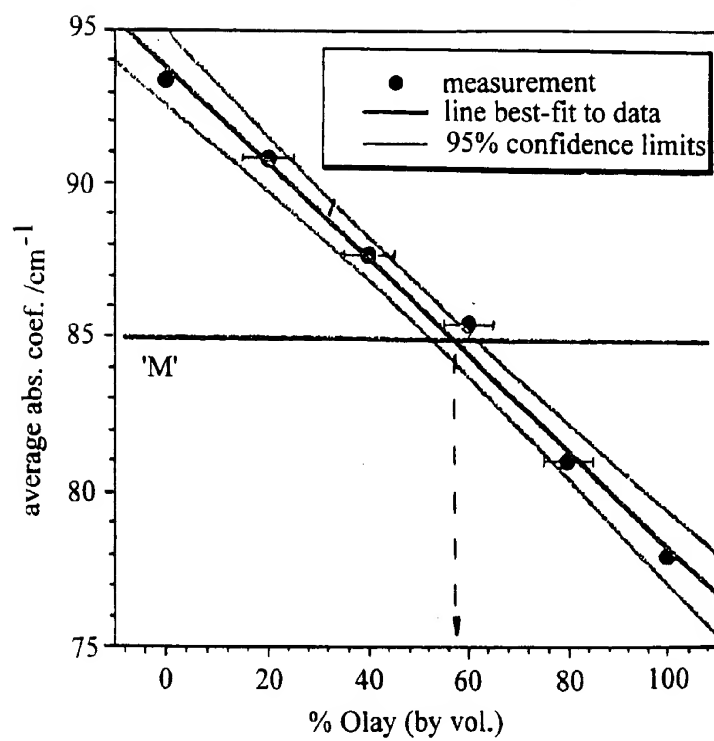


Fig. 49